


Oscilloscope HM407-2

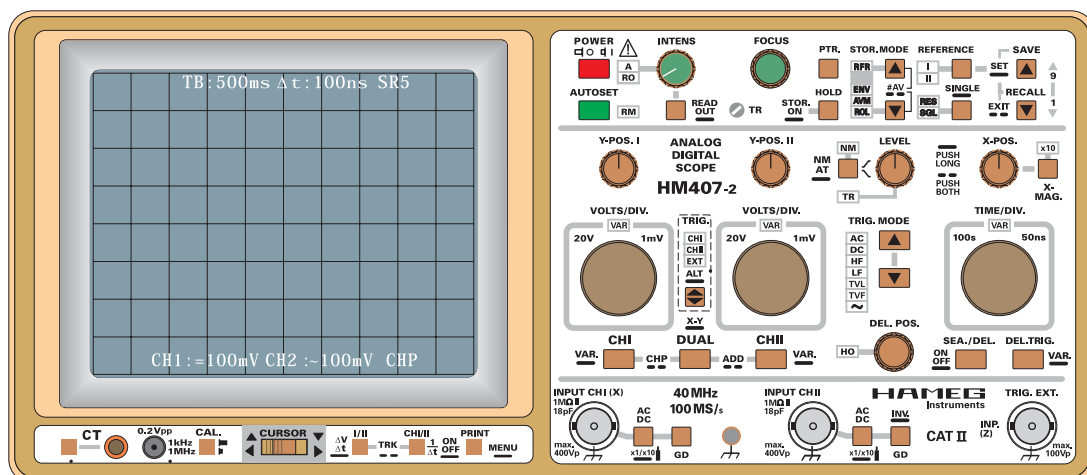

CE - Declaration of conformity 4

Technical Data 5

ATT 6

MB 10

YF 18

FC 20

DIGI 23

CCT 29

CRT 32

PS 34

IF 37



Herstellers
Manufacturer
Fabricant

HAMEG GmbH
Kelsterbacherstraße 15-19
D - 60528 Frankfurt

Bezeichnung / Product name / Designation:

Oszilloskop/Oscilloscope/Oscilloscope

Typ / Type / Type: HM407-2

mit / with / avec: -

Optionen / Options / Options: HO79-6

mit den folgenden Bestimmungen / with applicable regulations / avec les directives suivantes

EMV Richtlinie 89/336/EWG ergänzt durch 91/263/EWG, 92/31/EWG
EMC Directive 89/336/EEC amended by 91/263/EWG, 92/31/EEC
Directive EMC 89/336/CEE amendée par 91/263/EWG, 92/31/CEE

Niederspannungsrichtlinie 73/23/EWG ergänzt durch 93/68/EWG
Low-Voltage Equipment Directive 73/23/EEC amended by 93/68/EEC
Directive des équipements basse tension 73/23/CEE amendée par 93/68/CEE

KONFORMITÄTSERKLÄRUNG
DECLARATION OF CONFORMITY
DECLARATION DE CONFORMITE

HAMEG
Instruments

Angewendete harmonisierte Normen / Harmonized standards applied / Normes harmonisées utilisées

Sicherheit / Safety / Sécurité

EN 61010-1: 1993 / IEC (CEI) 1010-1: 1990 A 1: 1992 / VDE 0411: 1994
EN 61010-1/A2: 1995 / IEC 1010-1/A2: 1995 / VDE 0411 Teil 1/A1: 1996-05
Überspannungskategorie / Overvoltage category / Catégorie de surtension: II
Verschmutzungsgrad / Degree of pollution / Degré de pollution: 2

Elektromagnetische Verträglichkeit / Electromagnetic compatibility /
Compatibilité électromagnétique

EN 61326-1/A1

Störaussendung / Radiation / Emission: Tabelle / table / tableau 4; Klasse / Class /
Classe B.

Störfestigkeit / Immunity / Imunitee: Tabelle / table / tableau A1.

EN 61000-3-2/A14

Oberschwingungsströme / Harmonic current emissions / Émissions de courant
harmonique: Klasse / Class / Classe D.

EN 61000-3-3

Spannungsschwankungen u. Flicker / Voltage fluctuations and flicker /
Fluctuations de tension et du flicker.

Datum / Date / Date

15.01.2001

Unterschrift / Signature / Signatur

E. Baumgartner
Technical Manager / Directeur Technique

General information regarding the CE marking

HAMEG instruments fulfill the regulations of the EMC directive. The conformity test made by HAMEG is based on the actual generic- and product standards. In cases where different limit values are applicable, HAMEG applies the severer standard. For emission the limits for residential, commercial and light industry are applied. Regarding the immunity (susceptibility) the limits for industrial environment have been used.

The measuring- and data lines of the instrument have much influence on emission and immunity and therefore on meeting the acceptance limits. For different applications the lines and/or cables used may be different. For measurement operation the following hints and conditions regarding emission and immunity should be observed:

1. Data cables

For the connection between instruments resp. their interfaces and external devices, (computer, printer etc.) sufficiently screened cables must be used. Without a special instruction in the manual for a reduced cable length, the maximum cable length of a dataline must be less than 3 meters and not be used outside buildings. If an interface has several connectors only one connector must have a connection to a cable.

Basically interconnections must have a double screening. For IEEE-bus purposes the double screened cables HZ72S and HZ72L from HAMEG are suitable.

2. Signal cables

Basically test leads for signal interconnection between test point and instrument should be as short as possible. Without instruction in the manual for a shorter length, signal lines must be less than 3 meters and not be used outside buildings.

Signal lines must be screened (coaxial cable - RG58/U). A proper ground connection is required. In combination with signal generators double screened cables (RG223/U, RG214/U) must be used.

3. Influence on measuring instruments.

Under the presence of strong high frequency electric or magnetic fields, even with careful setup of the measuring equipment an influence of such signals is unavoidable.

This will not cause damage or put the instrument out of operation. Small deviations of the measuring value (reading) exceeding the instruments specifications may result from such conditions in individual cases.

4. RF immunity of oscilloscopes.

4.1 Electromagnetic RF field

The influence of electric and magnetic RF fields may become visible (e.g. RF superimposed), if the field intensity is high. In most cases the coupling into the oscilloscope takes place via the device under test, mains/line supply, test leads, control cables and/or radiation. The device under test as well as the oscilloscope may be effected by such fields.

Although the interior of the oscilloscope is screened by the cabinet, direct radiation can occur via the CRT gap. As the bandwidth of each amplifier stage is higher than the total -3dB bandwidth of the oscilloscope, the influence RF fields of even higher frequencies may be noticeable.

4.2 Electrical fast transients / electrostatic discharge

Electrical fast transient signals (burst) may be coupled into the oscilloscope directly via the mains/line supply, or indirectly via test leads and/or control cables. Due to the high trigger and input sensitivity of the oscilloscopes, such normally high signals may effect the trigger unit and/or may become visible on the CRT, which is unavoidable. These effects can also be caused by direct or indirect electrostatic discharge.

HAMEG GmbH

Specifications

Vertical Deflection

Operating modes: Channel I or CH II separate, Channel I and II: alternate or chopped (Chopper Frequency approx. 0.5MHz)
Sum or Difference from Channel I and $\pm$ Ch. II,
XY-Mode: via CH I (X) and CH II (Y).
Frequency range: 2x DC to 40MHz (-3dB).
 Risettime: <8.75ns. Overshoot: $\leq 1\%$.
Deflection coefficient: 14 calibrated positions variable 2.5:1 to min. **50V/div.**
1mV/div and 2mV/div: $\pm 5\%$ (0 to 10MHz (-3dB))
5mV/div to 20V/div: $\pm 3\%$ (1-2-5sequence).
Input impedance: 1M Ω || 18pF.
 Input coupling: DC - AC - GD (Ground)
 Input voltage: max. 400V (DC + peak AC).

Triggering

Automatic(peak to peak): **$\leq 20\text{Hz}$ -100MHz**($\geq 0.5\text{div}$),
 Normal: **DC-100MHz**, LED for trigger indication.
Slope: positive or negative.
Sources: CH I or II, line, ext.
 CH I alternate CH II ($\geq 0.8\text{div}$).
 Coupling: **AC** ($\geq 10\text{Hz}$ - 100MHz), **DC** (0 - 100MHz),
HF (50kHz - 100MHz), **LF** (0 - $\leq 1.5\text{kHz}$).
Triggering ext.: $\geq 0.3V_{pp}$ from DC to 40MHz
Active TV-Sync-Separator (field & line, pos, neg.)
2nd triggering (Del. Trig.): normal with level control DC to 100 MHz.

Horizontal Deflection

Time coefficients: 1-2-5 sequence, Accuracy $\pm 3\%$
Analog: 22 cal. positions from **0.5s - 50ns/div.**
Digital: 27 cal. positions from **100s - 0.2 μ s/div.**
 Variable (analog) 2.5:1 up to 1.25s/div.
X-MAG. x10: analog to 10ns/div., dig. to 20ns/div $\pm 5\%$.
Delay: 120ms - 200ns, variable,
Hold-off time (analog): variable to approx. 10:1.
Bandwidth X-amplifier (analog): 0-3MHz (-3dB).
 Input X-amplifier via Channel II, Sensitivity see Channel II.
X-Y-phase shift : $< 3^\circ$ below 120kHz.

Digital Storage

Operating modes: Refresh, Roll, Single, XY, Envelope, Average (2 to 512 waveforms).
Automatic Dot Join function
Sample Rate: max. **100MSa/s** (8 bit)
Refresh rate: max. 180/s
Record length: 2048 x 8 bit per channel.
Reference memory: 2 x 2k x 8bit (EEPROM).
Resolution: Y: **25 points/div**, X: **200 points/div**.
Pre-/Posttriggerer: 25, 50, 75, 100, -25, -50, -75%.

Operation / Control

Manual (front panel switches);
Auto Set (automatic parameter selection).
Save / Recall of 9 user-defined parameter settings
RS232 interface for remote control via a PC.
 Remote control (Option) **HZ68**.
Multifunction-Interface HO79-6(Option): RS232, IEEE-488, Centronics (Postscript, HPGL, PCL, EPSON).
Readout: Display of parameter settings.
Cursor measurement of ΔV , Δt or $\Delta 1/t$ (frequency), separate or in tracking mode.


Component Tester

Test voltage: approx. 7V_{rms} (open circuit).
Test current: max. 7mA_{rms} (short circuit).
Test frequency: approx. 50Hz
 One test lead is grounded (Safety Earth).

General Information

CRT: D14-364GY/123 or ER151-GH/-, rectangular screen (8x10cm) internal graticule
Acceleration voltage: approx 2000V
Trace rotation: adjustable on front panel
Calibrator: square-wave generator ($t_r < 4\text{ns}$) $\approx 1\text{kHz}/1\text{MHz}$; Output: 0.2V $\pm 1\%$.
Analog Intensitymodulation, max. +5V (TTL).
Line voltage: 100-240V AC $\pm 10\%$, 50/60Hz
Power consumption: approx. 42 Watt at 50Hz.
 Min./Max. ambient temperature: 0°C...+40°C
Protective system: Safety class I (IEC1010-1)
 Weight: approx. 6.0kg, color: techno-brown
 Cabinet: W 285, H 125, D 380 mm

4/00

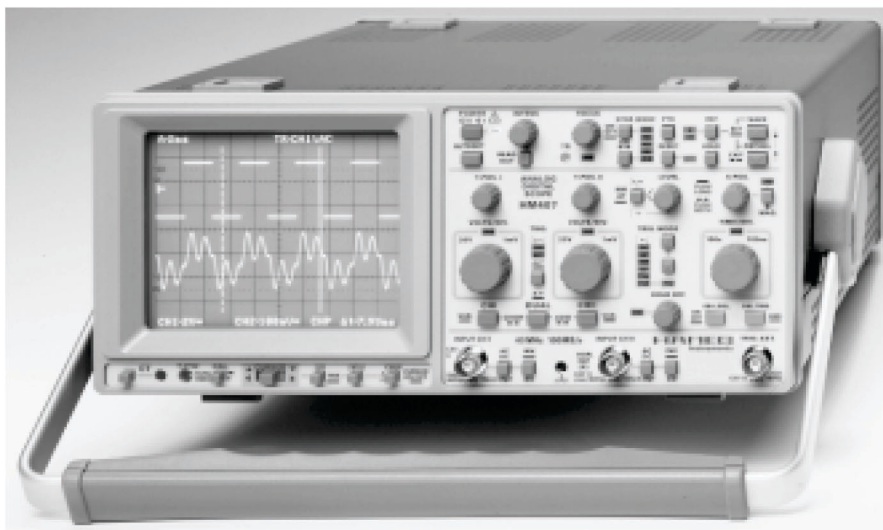

40MHz Analog-/Digital-Scope HM407-2

Auto-Set, Save/Recall, Readout/Cursor, RS232 Interface

Analog: 2 x DC-40MHz, max. 1mV/div, Timebase 0.5s/div - 10ns/div
Triggering DC - 100MHz, Component Tester, 1MHz Calibrator
Digital: Max. Sampling Rate 100MSa/s, Timebase 100s/div - 20ns/div
Storage 2 x 2048 x 8 bit, Reference Memory, Post/Pre-Trigger
Storage Modes: Refresh, Single, Roll, Average and Envelope

The worldwide success of HAMEG's HM205 and HM305 has led to the introduction of the new microprocessor controlled HM407-2 Analog/Digital oscilloscope. This instrument offers much more performance and specifications over its predecessors. The HM407-2 incorporates a microprocessor-based system that extensively automates operation. The majority of signals can be displayed by simply pressing the "Autoset" button. A "Save/Recall" function is available for storing frequently used setup parameters.

The increased maximum sampling rate of 100MSa/s now allows to capture a 10MHz signal in "Single" mode with 10 samples (dots) per period. The automatic Dot-Join function provides linear connections between the captured points, ensuring that all digitized signals are displayed without gaps. New features are the two reference memories, allowing their contents to be compared with the live signal at any time. Cursors can be activated for waveform measurements. All important parameter settings are displayed on the CRT screen. The built-in RS232-Interface enables remote control operation and signal processing via a PC.


Unique in its price range is also the analog section of the HM407-2. The increased bandwidth of 40MHz (-3dB) allows the stable display of signals up to 100MHz. As always, the Component Tester with one-button control is a standard feature in the HM407-2. This is also true for the switchable 1kHz/1MHz Calibrator which permits you to check the transient characteristics from probe tip to the screen at any time.

All in all, the new HM407-2 presents itself as a practical hands-on oscilloscope for today's progressive measurement requirements offering a price/performance ratio that sets new standards world-wide.


Accessories supplied:

Line Cord, Operators Manual and PC software on CD-ROM, 2 Probes 1:1/ 10:1

Screen photo of stored sinewave signals.

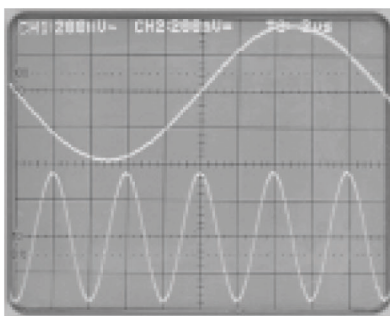



Screen shot of measurement software.

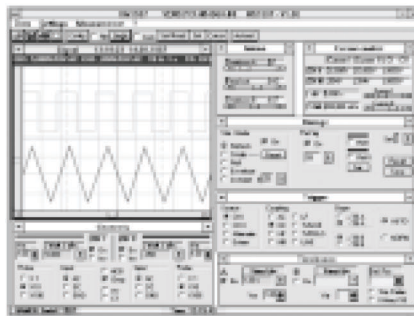






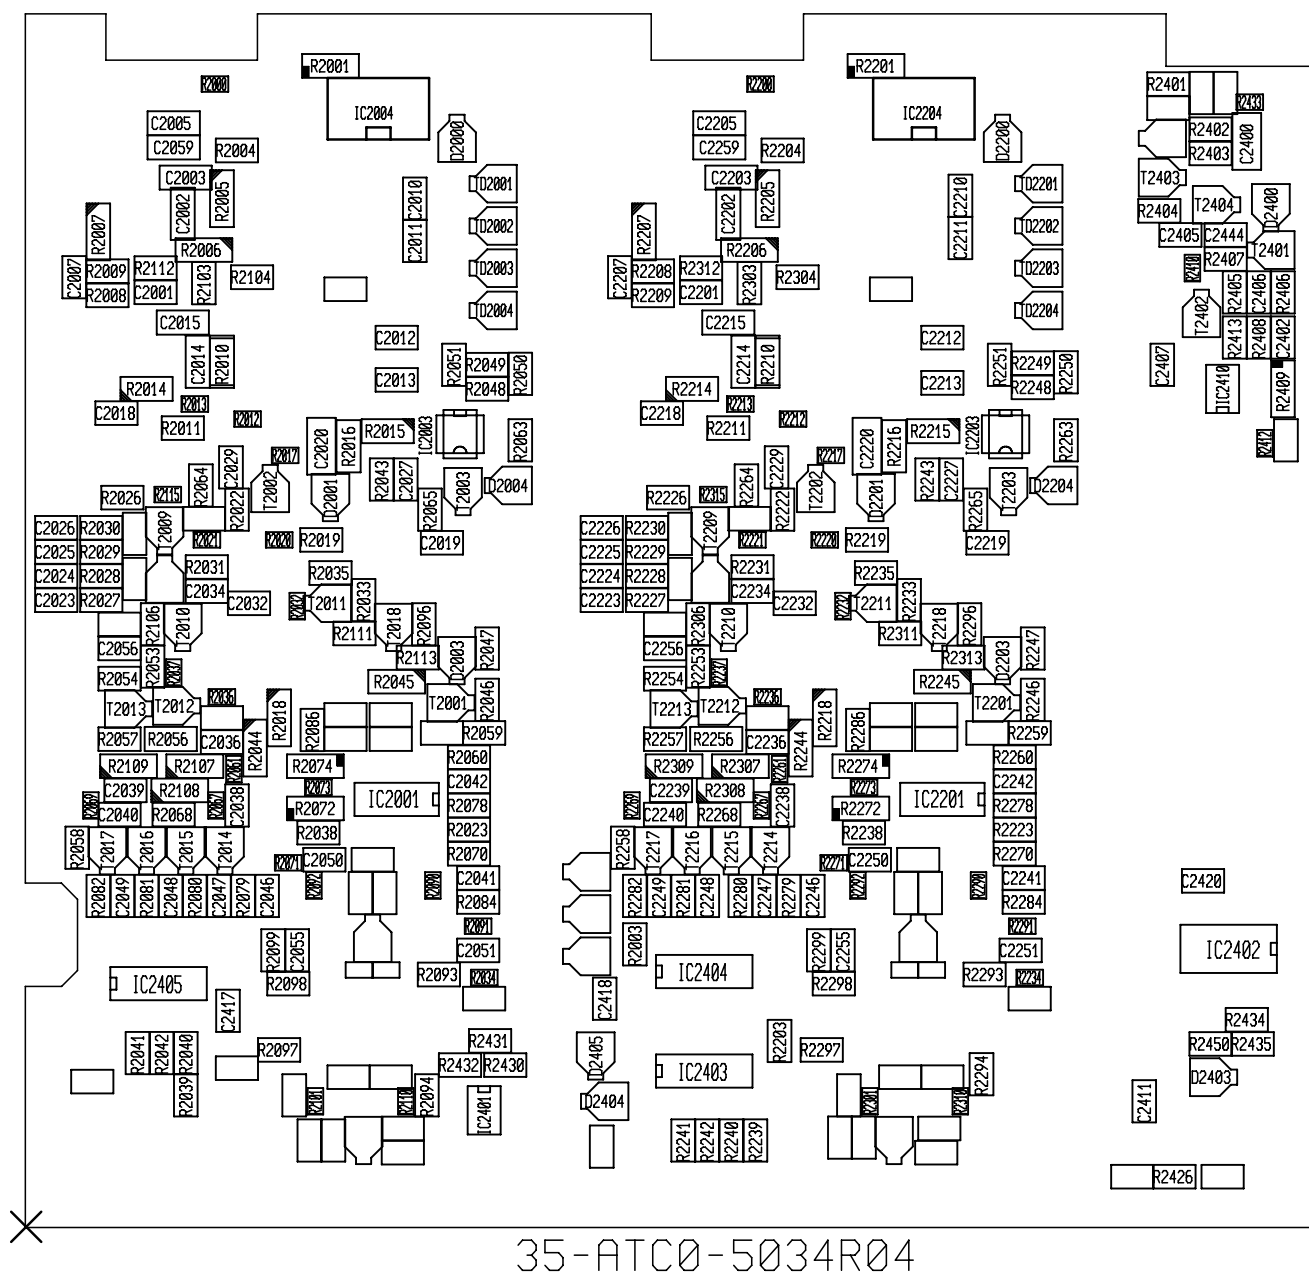

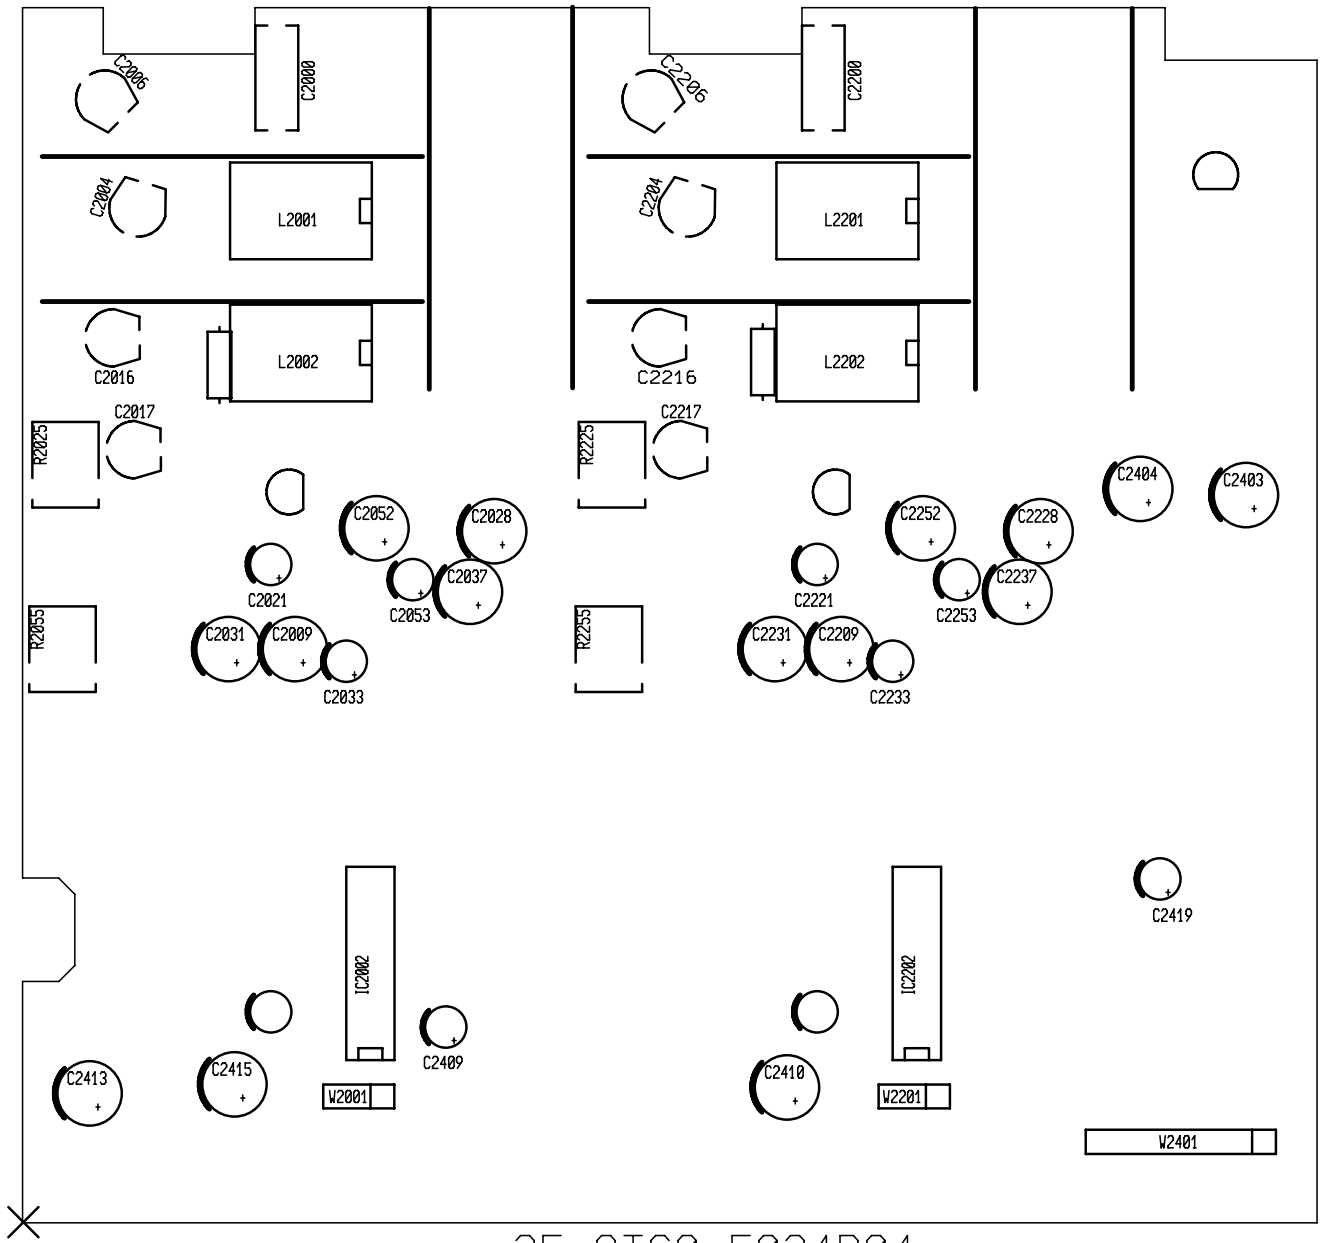


35-ATC0-5034R04

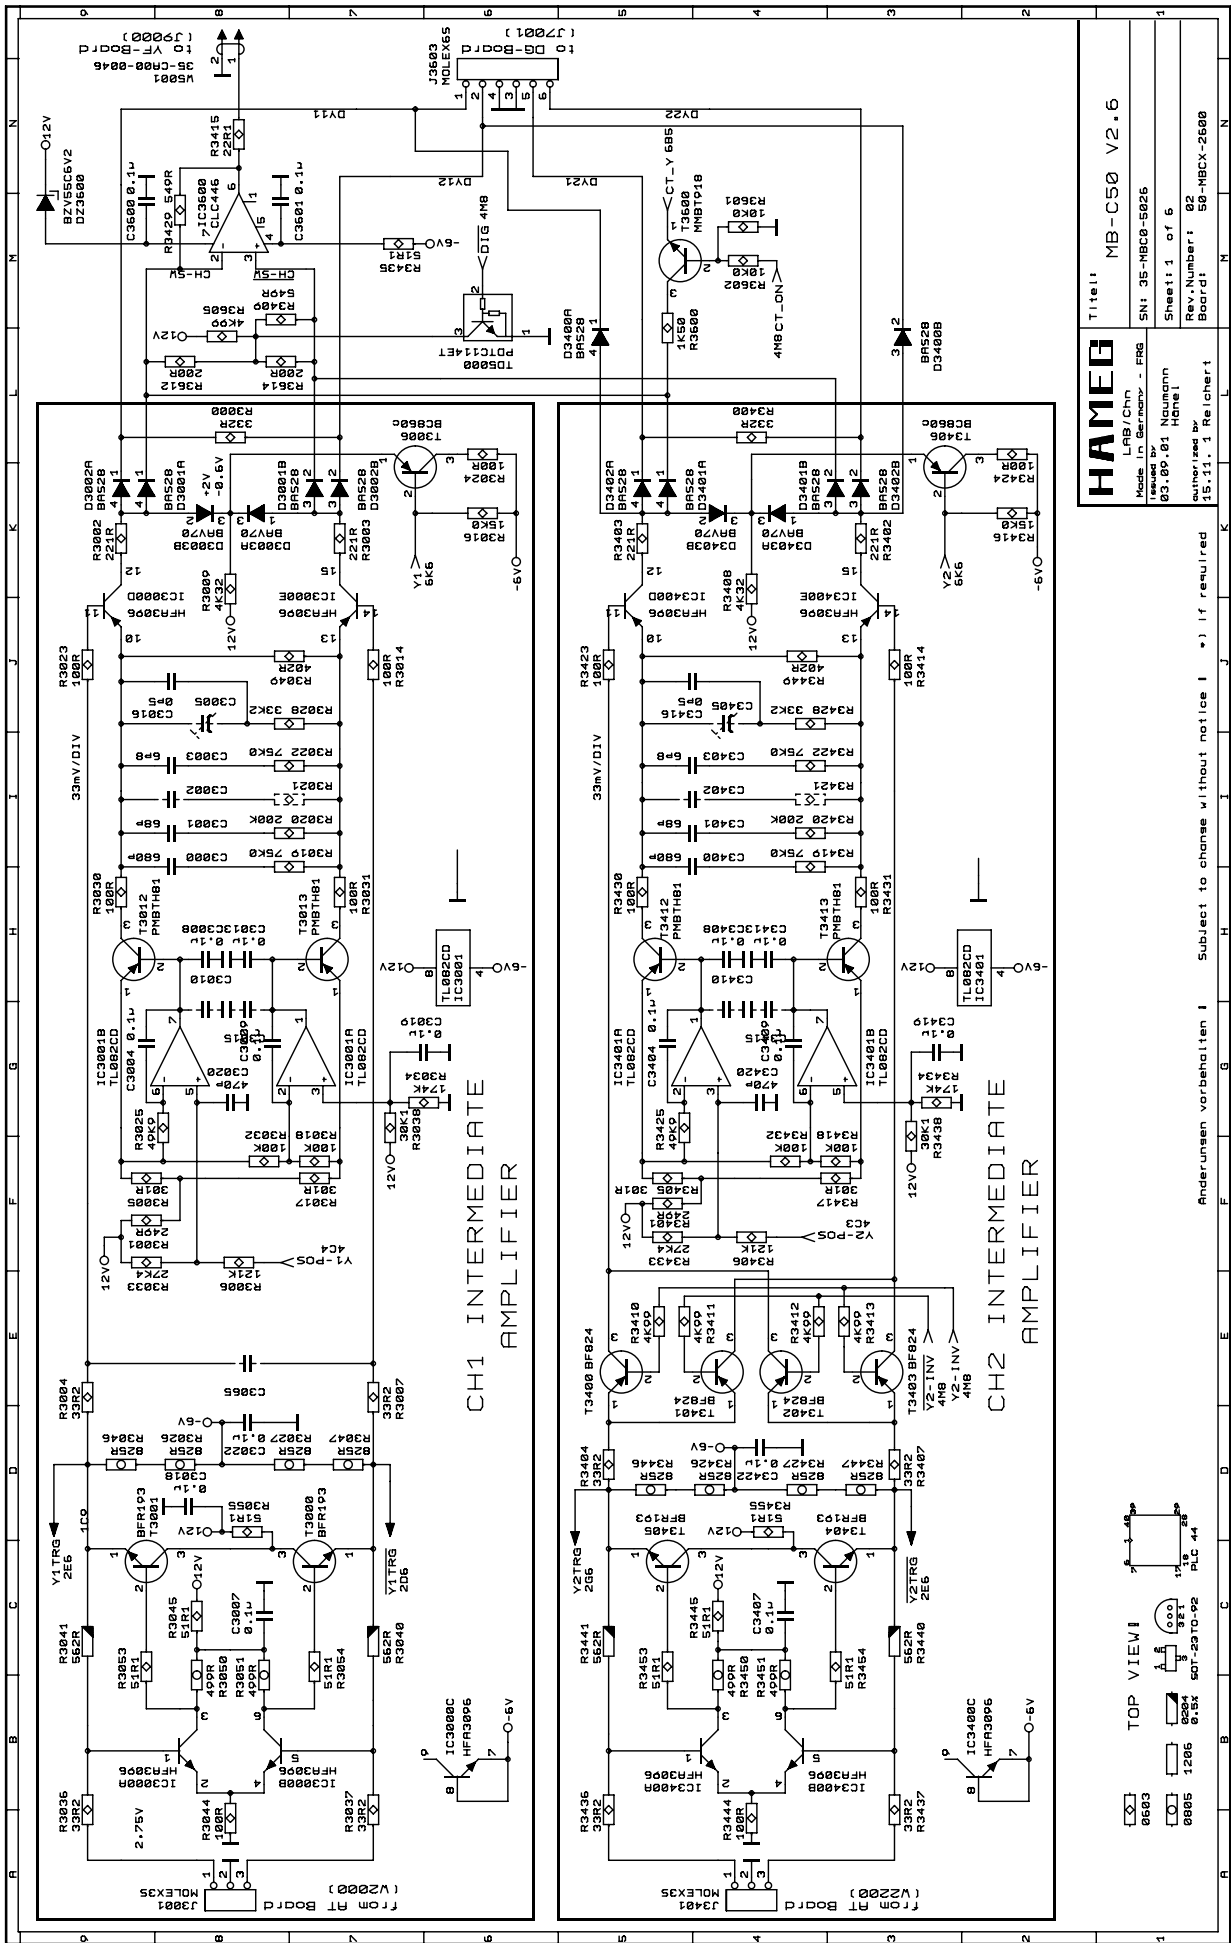


HAMEG	
Lab/Chn	MB-C50 V2.6
Made in Germany - FRG	SN: 35-HBC0-5026
Issued by	Sheet 1 of 6
03.09.01 Naumann	Rev. Number: 02
Authorized by	Board: 50-MBCX-2600
15.11.1 Reichert	


Subject to change without notice ! * If required




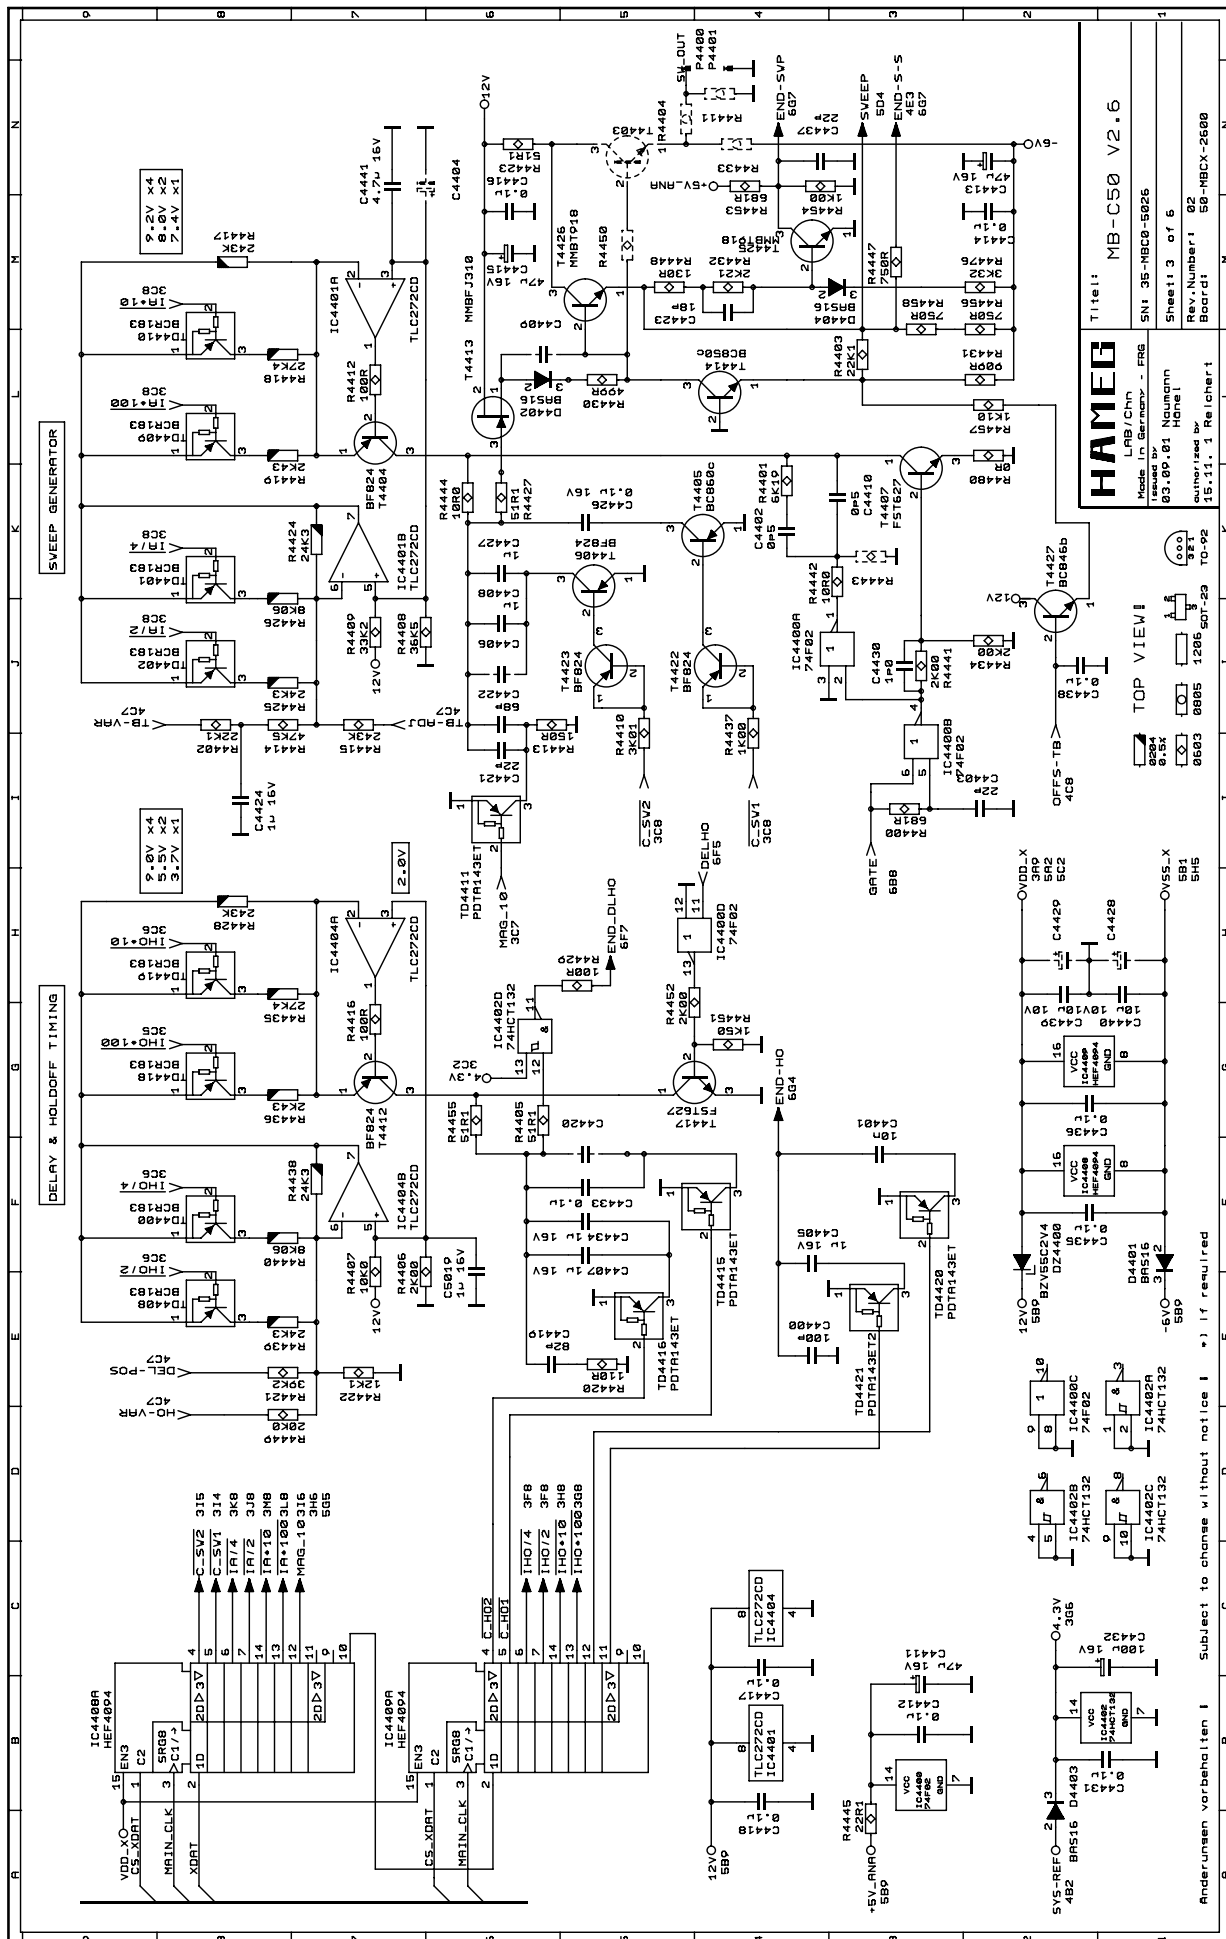




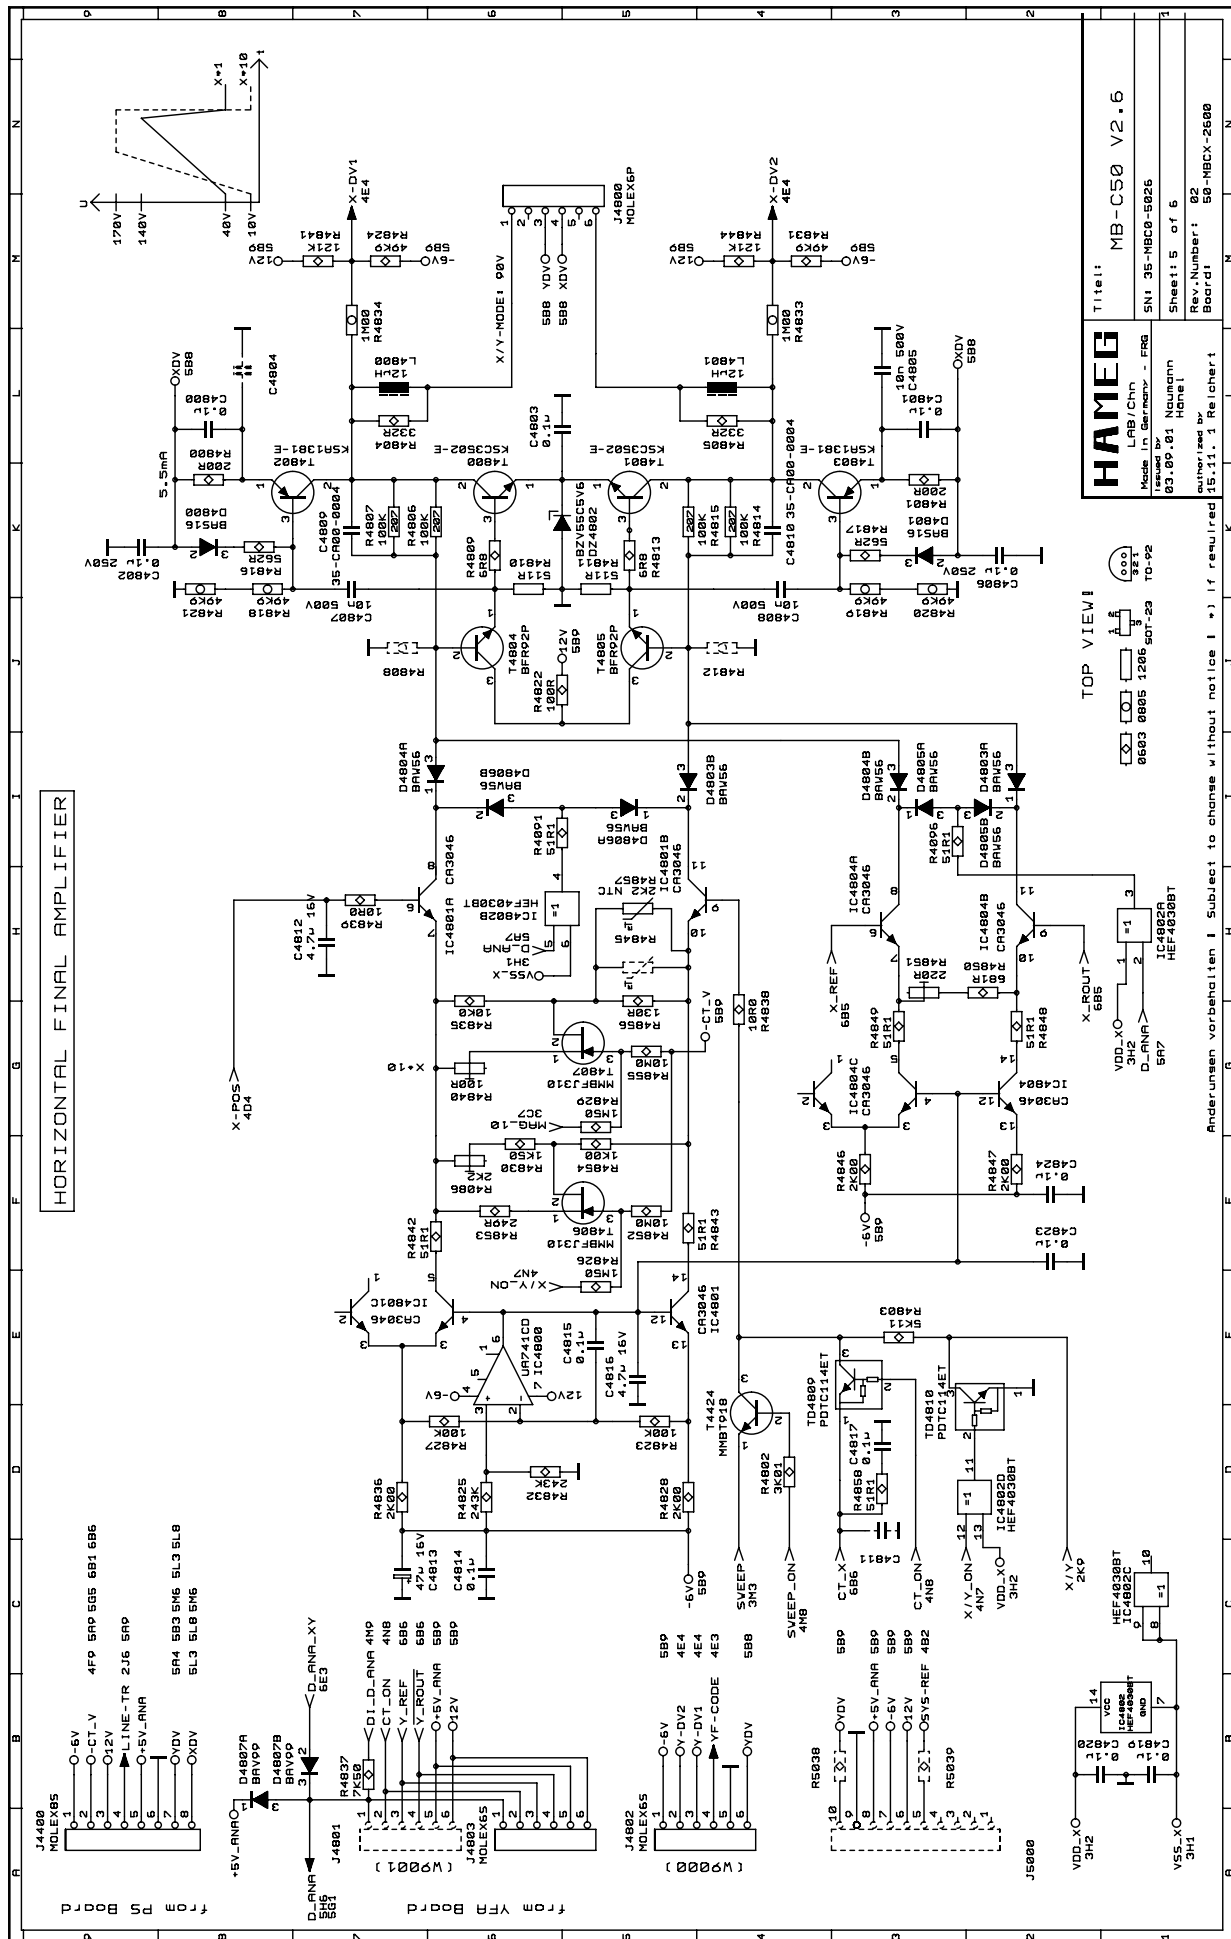


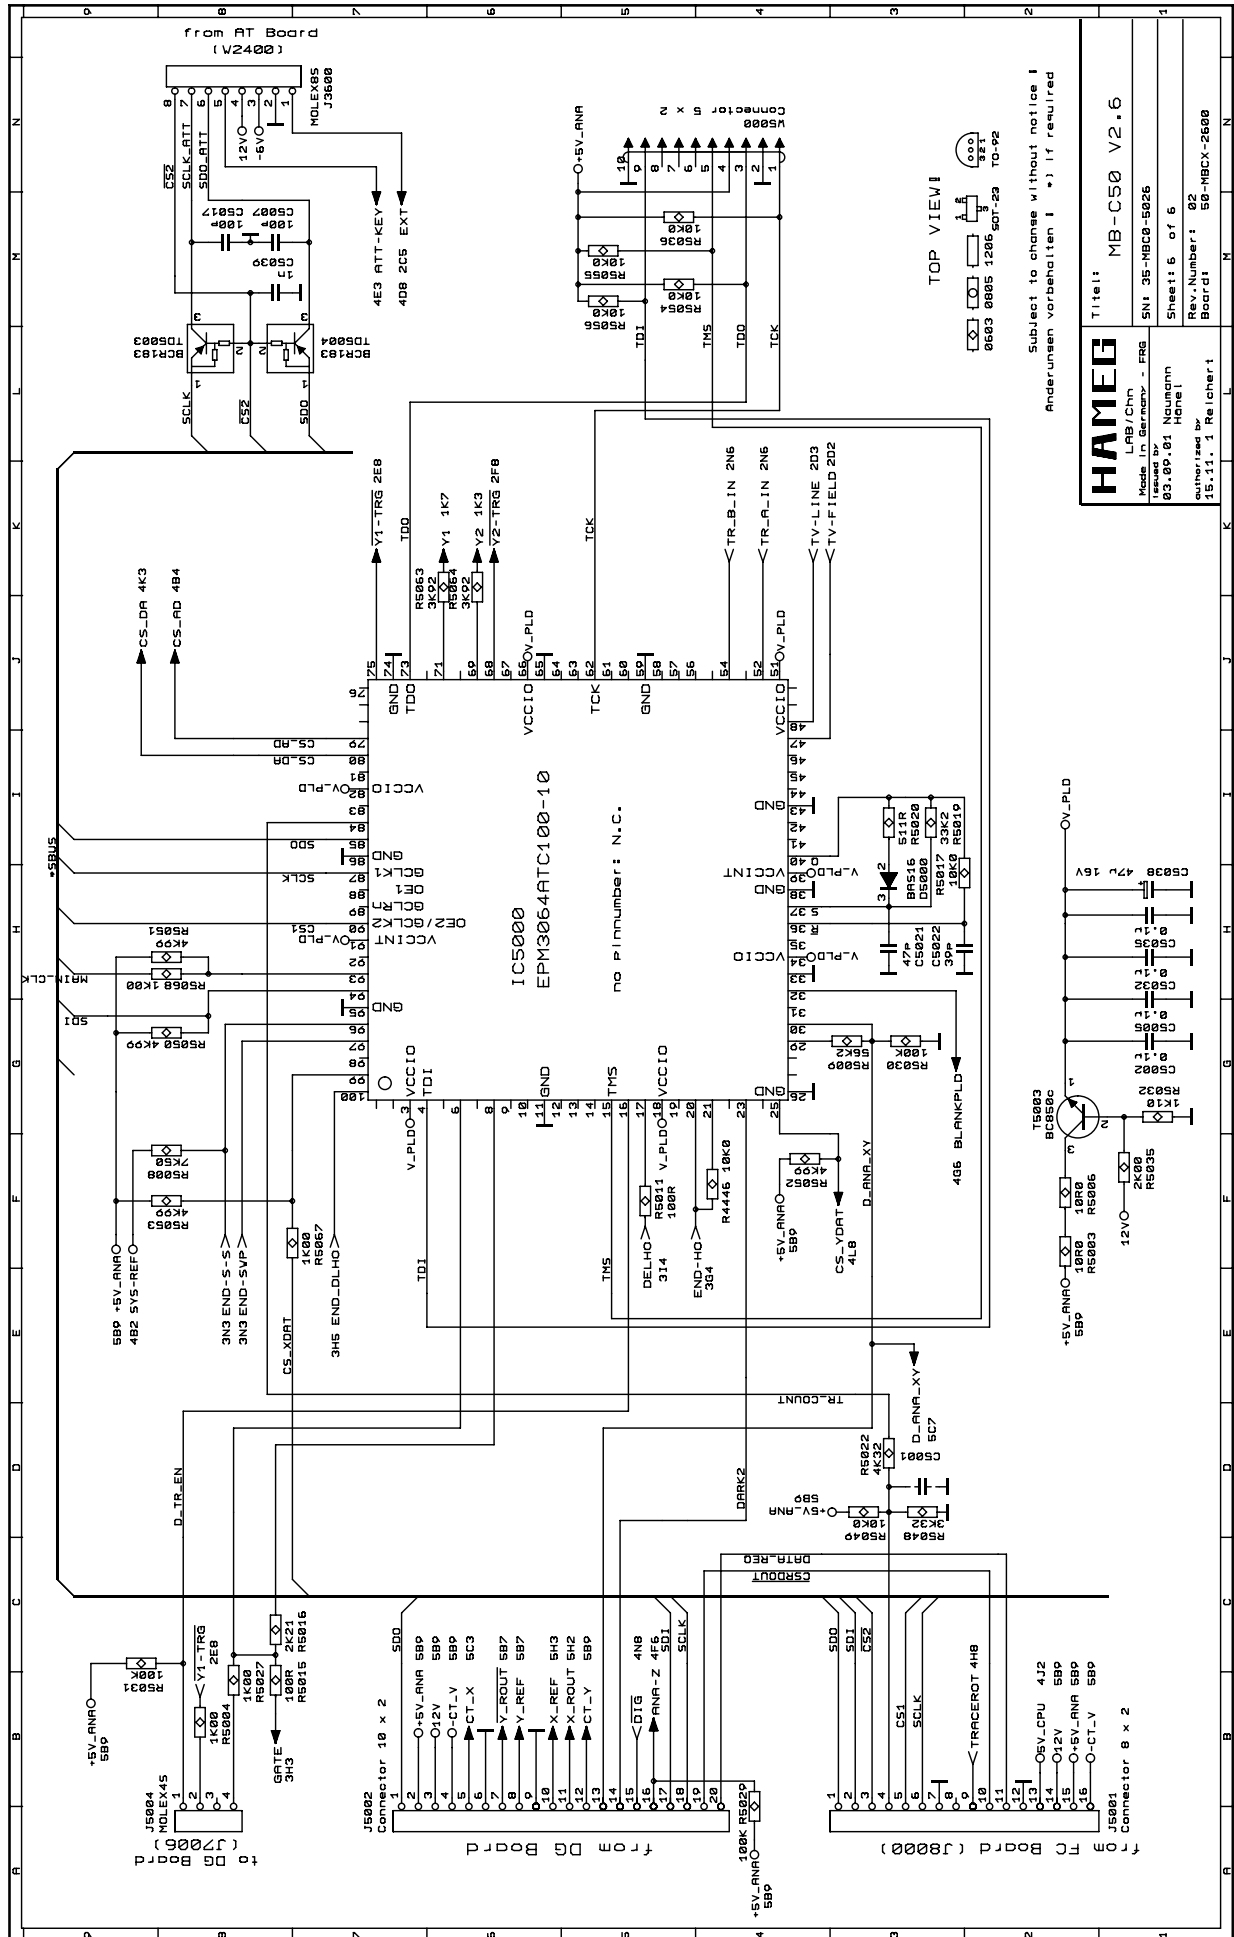


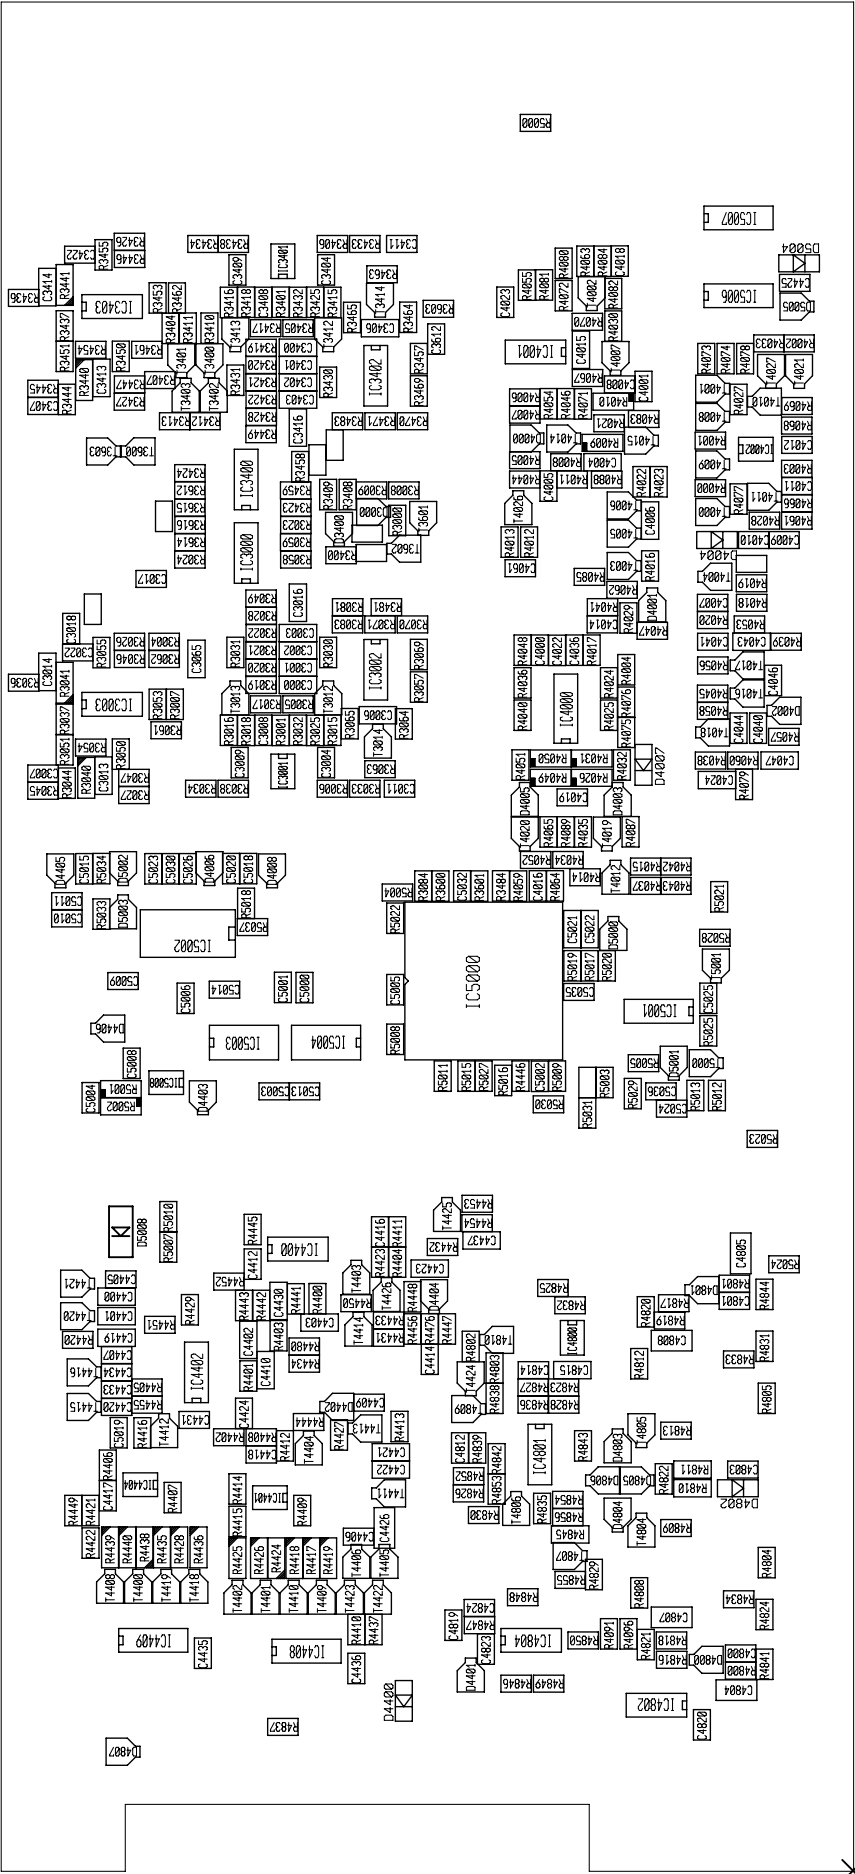


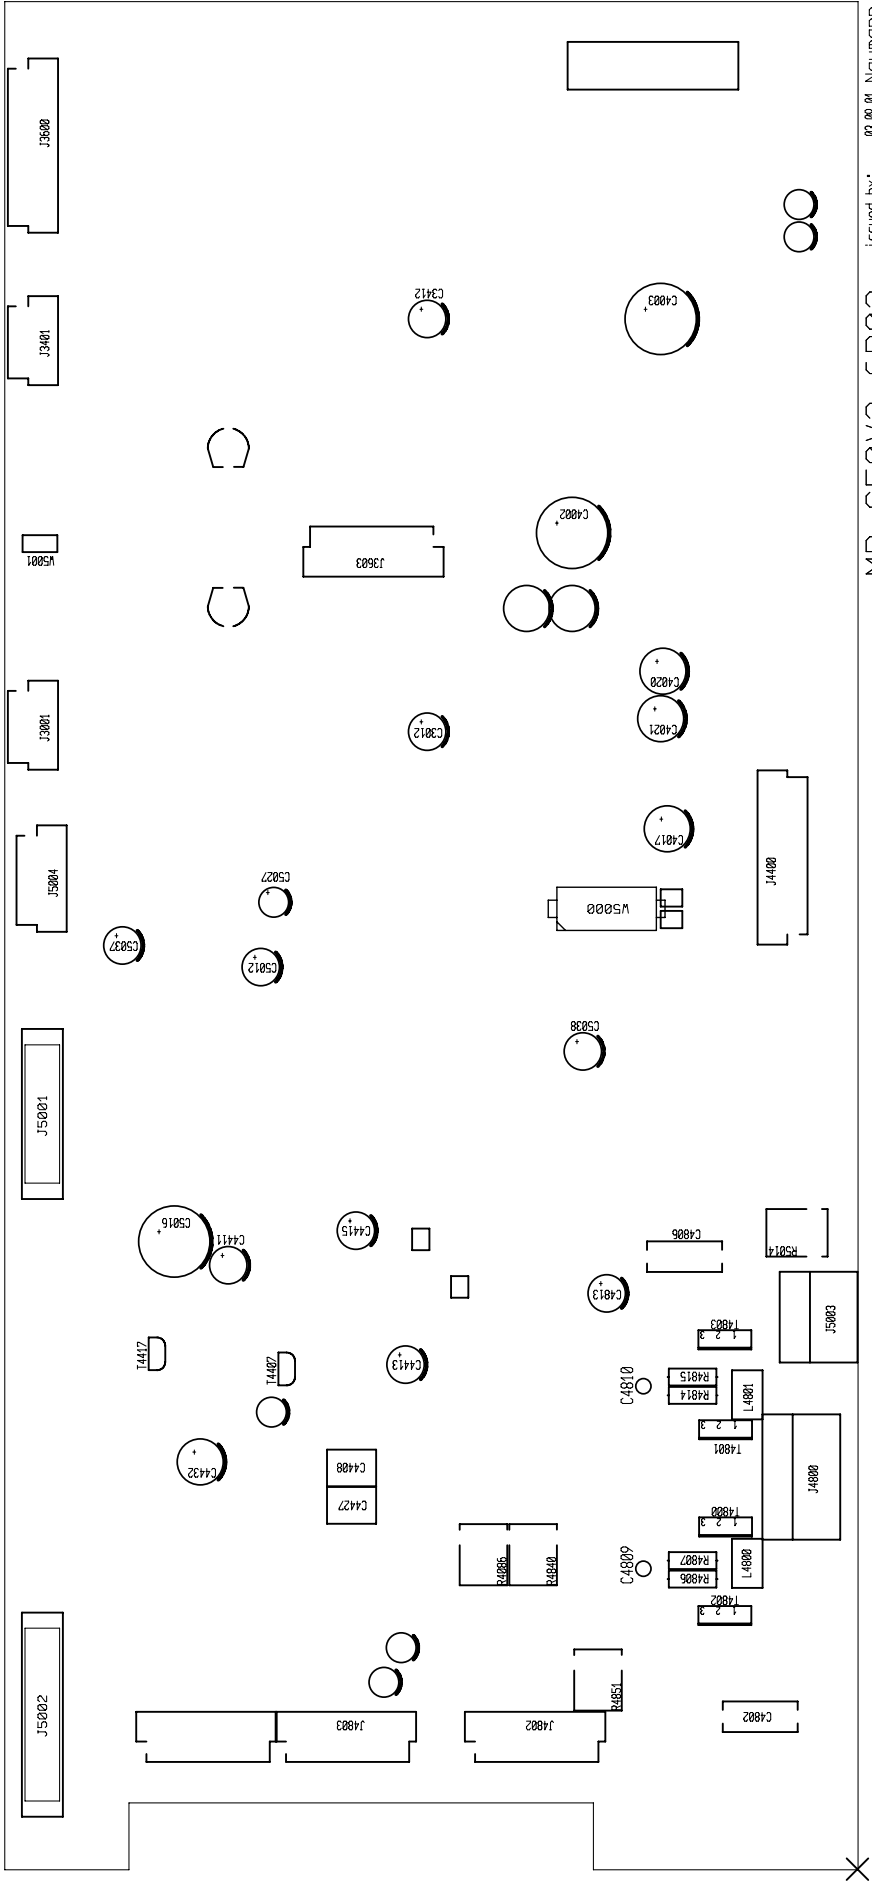



MB-C50V2.6R02 issued by: Naumann Hotel

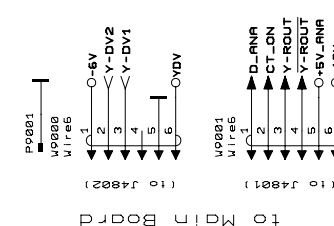


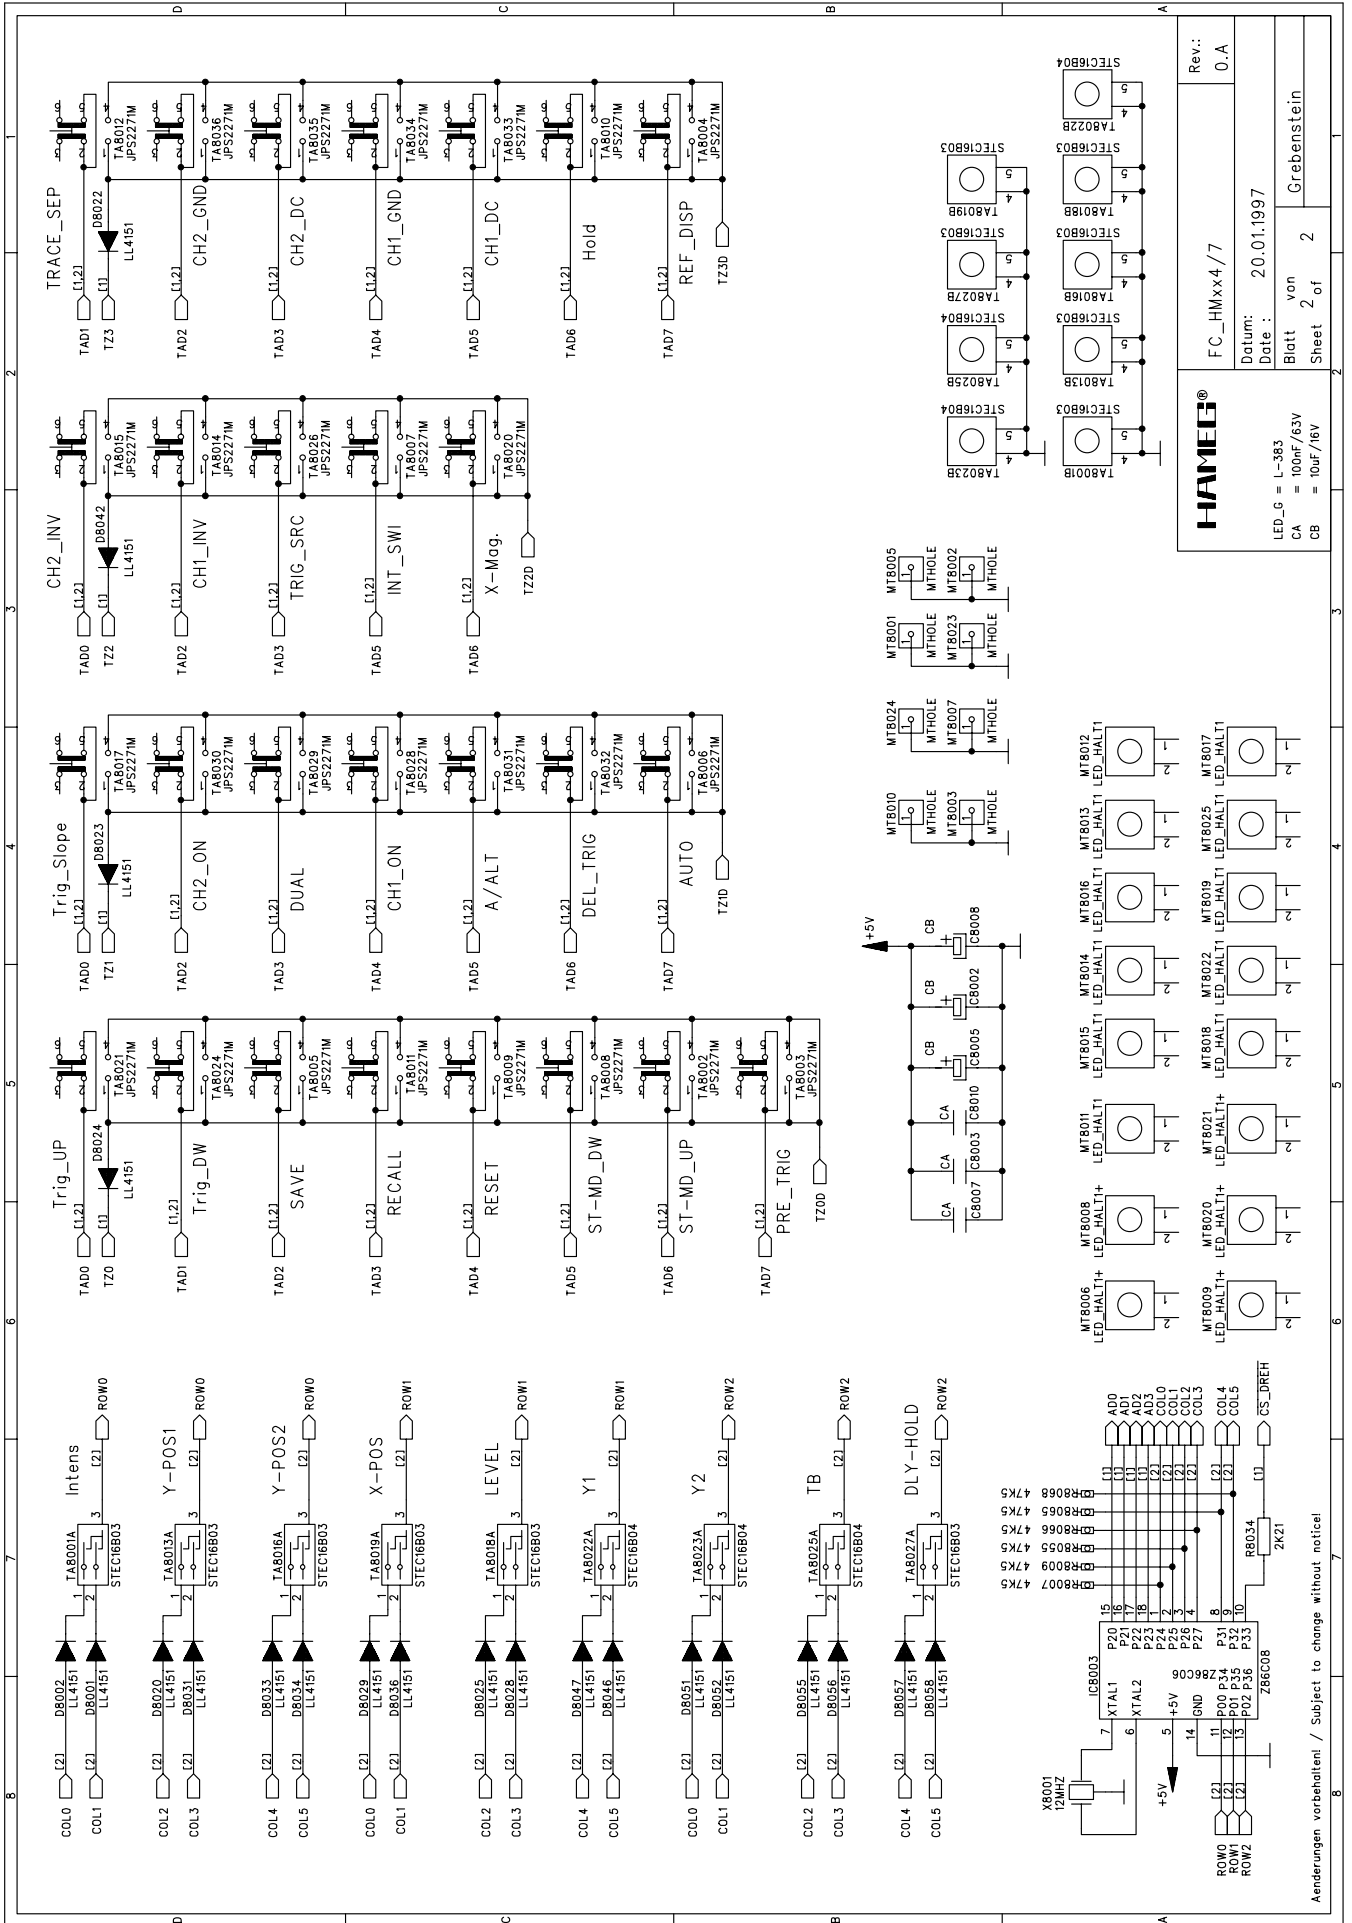

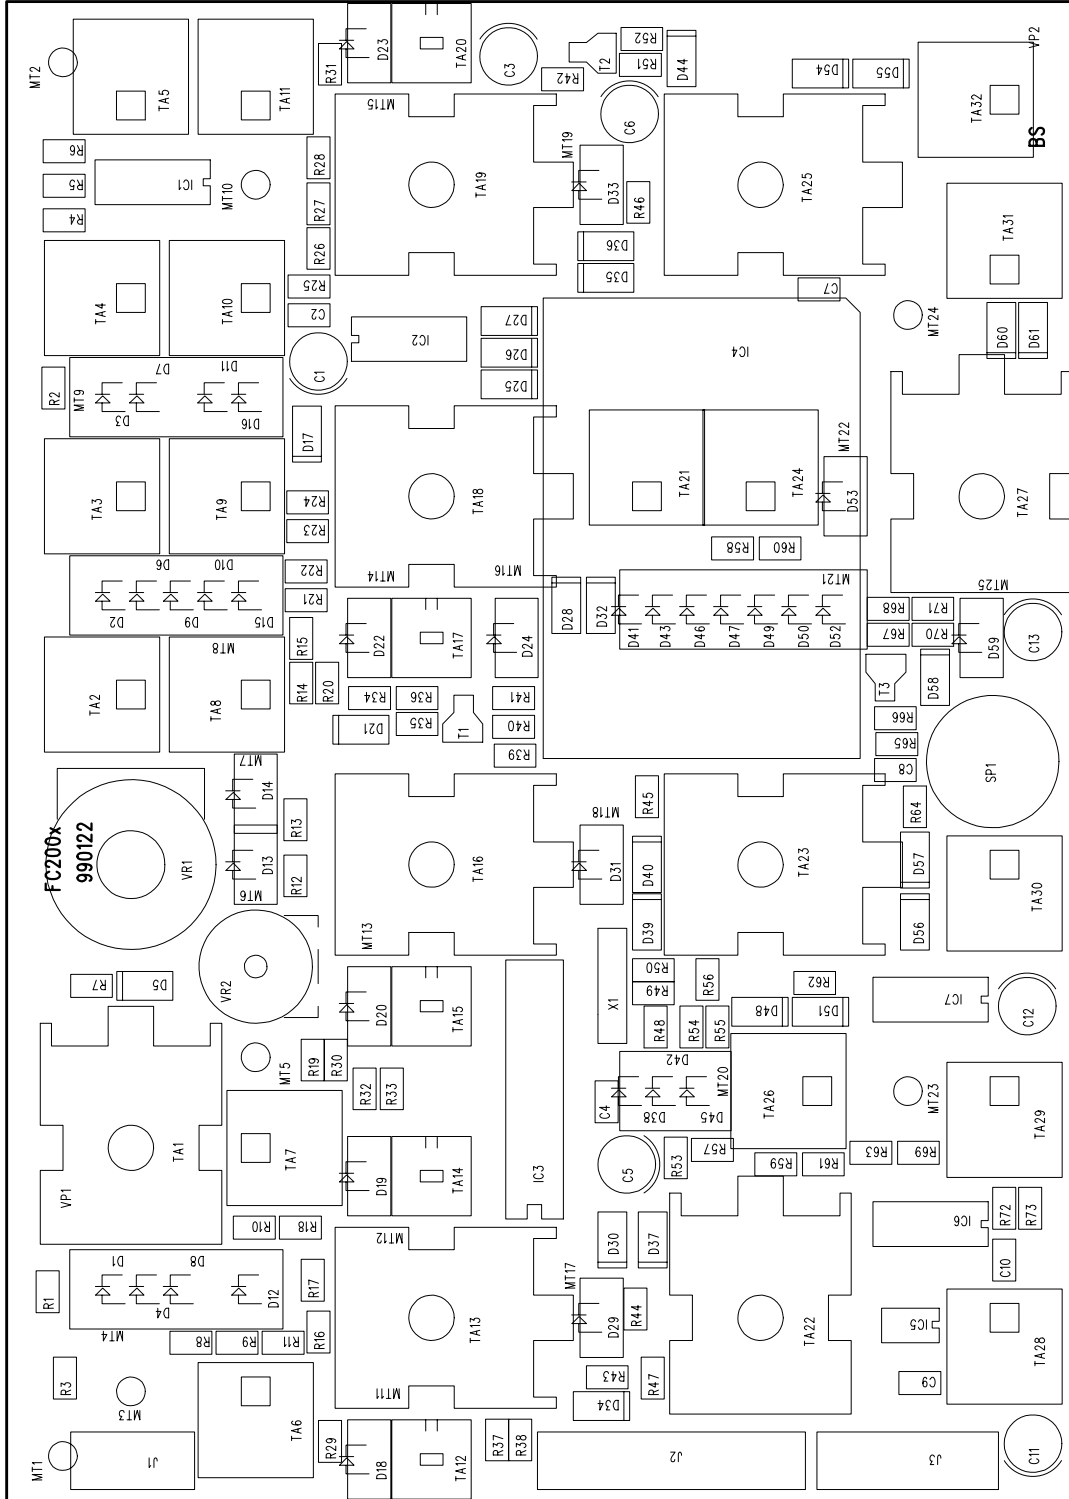

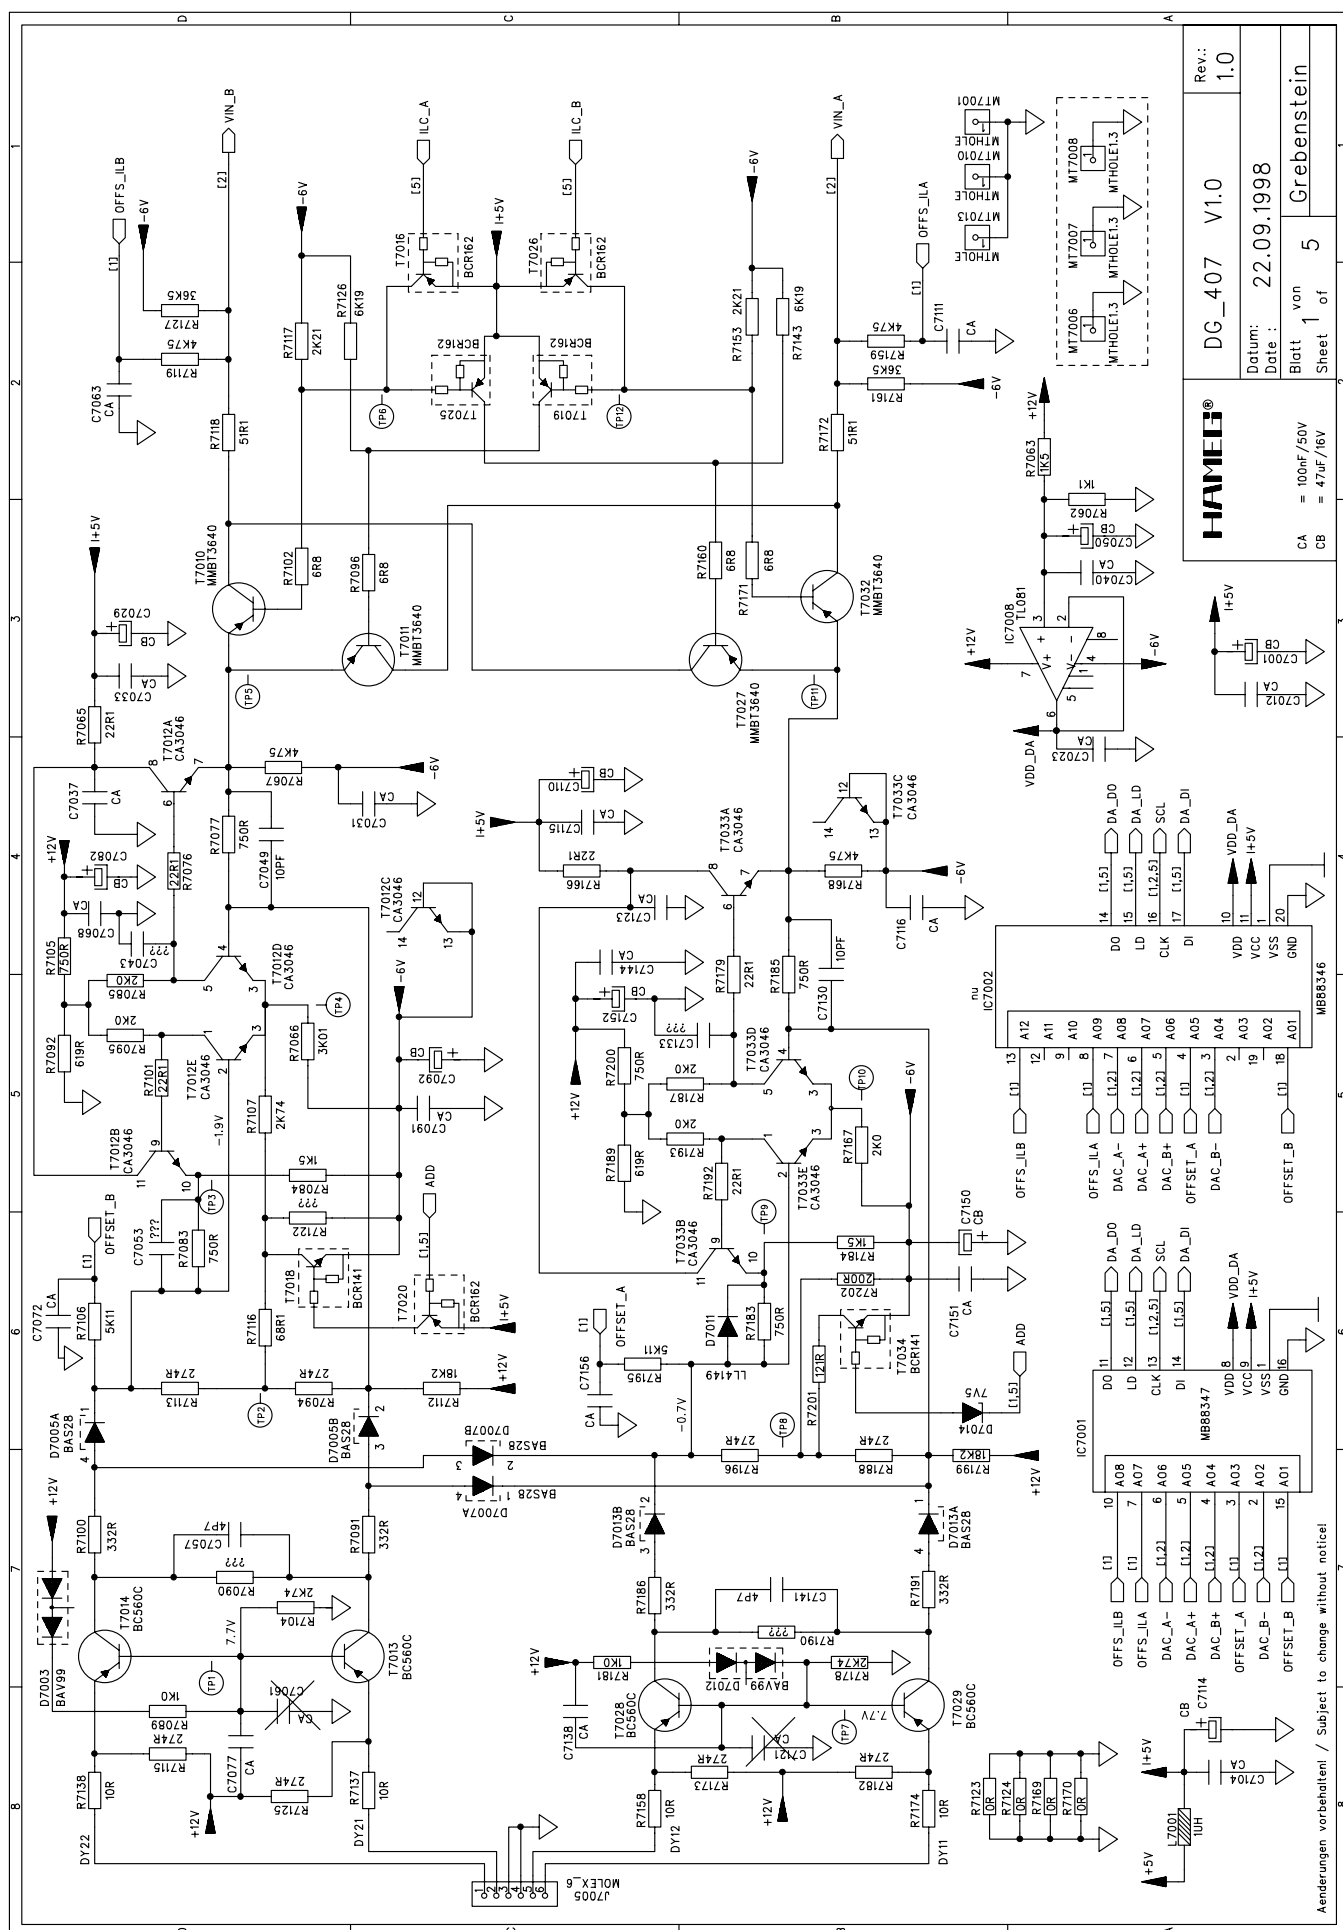



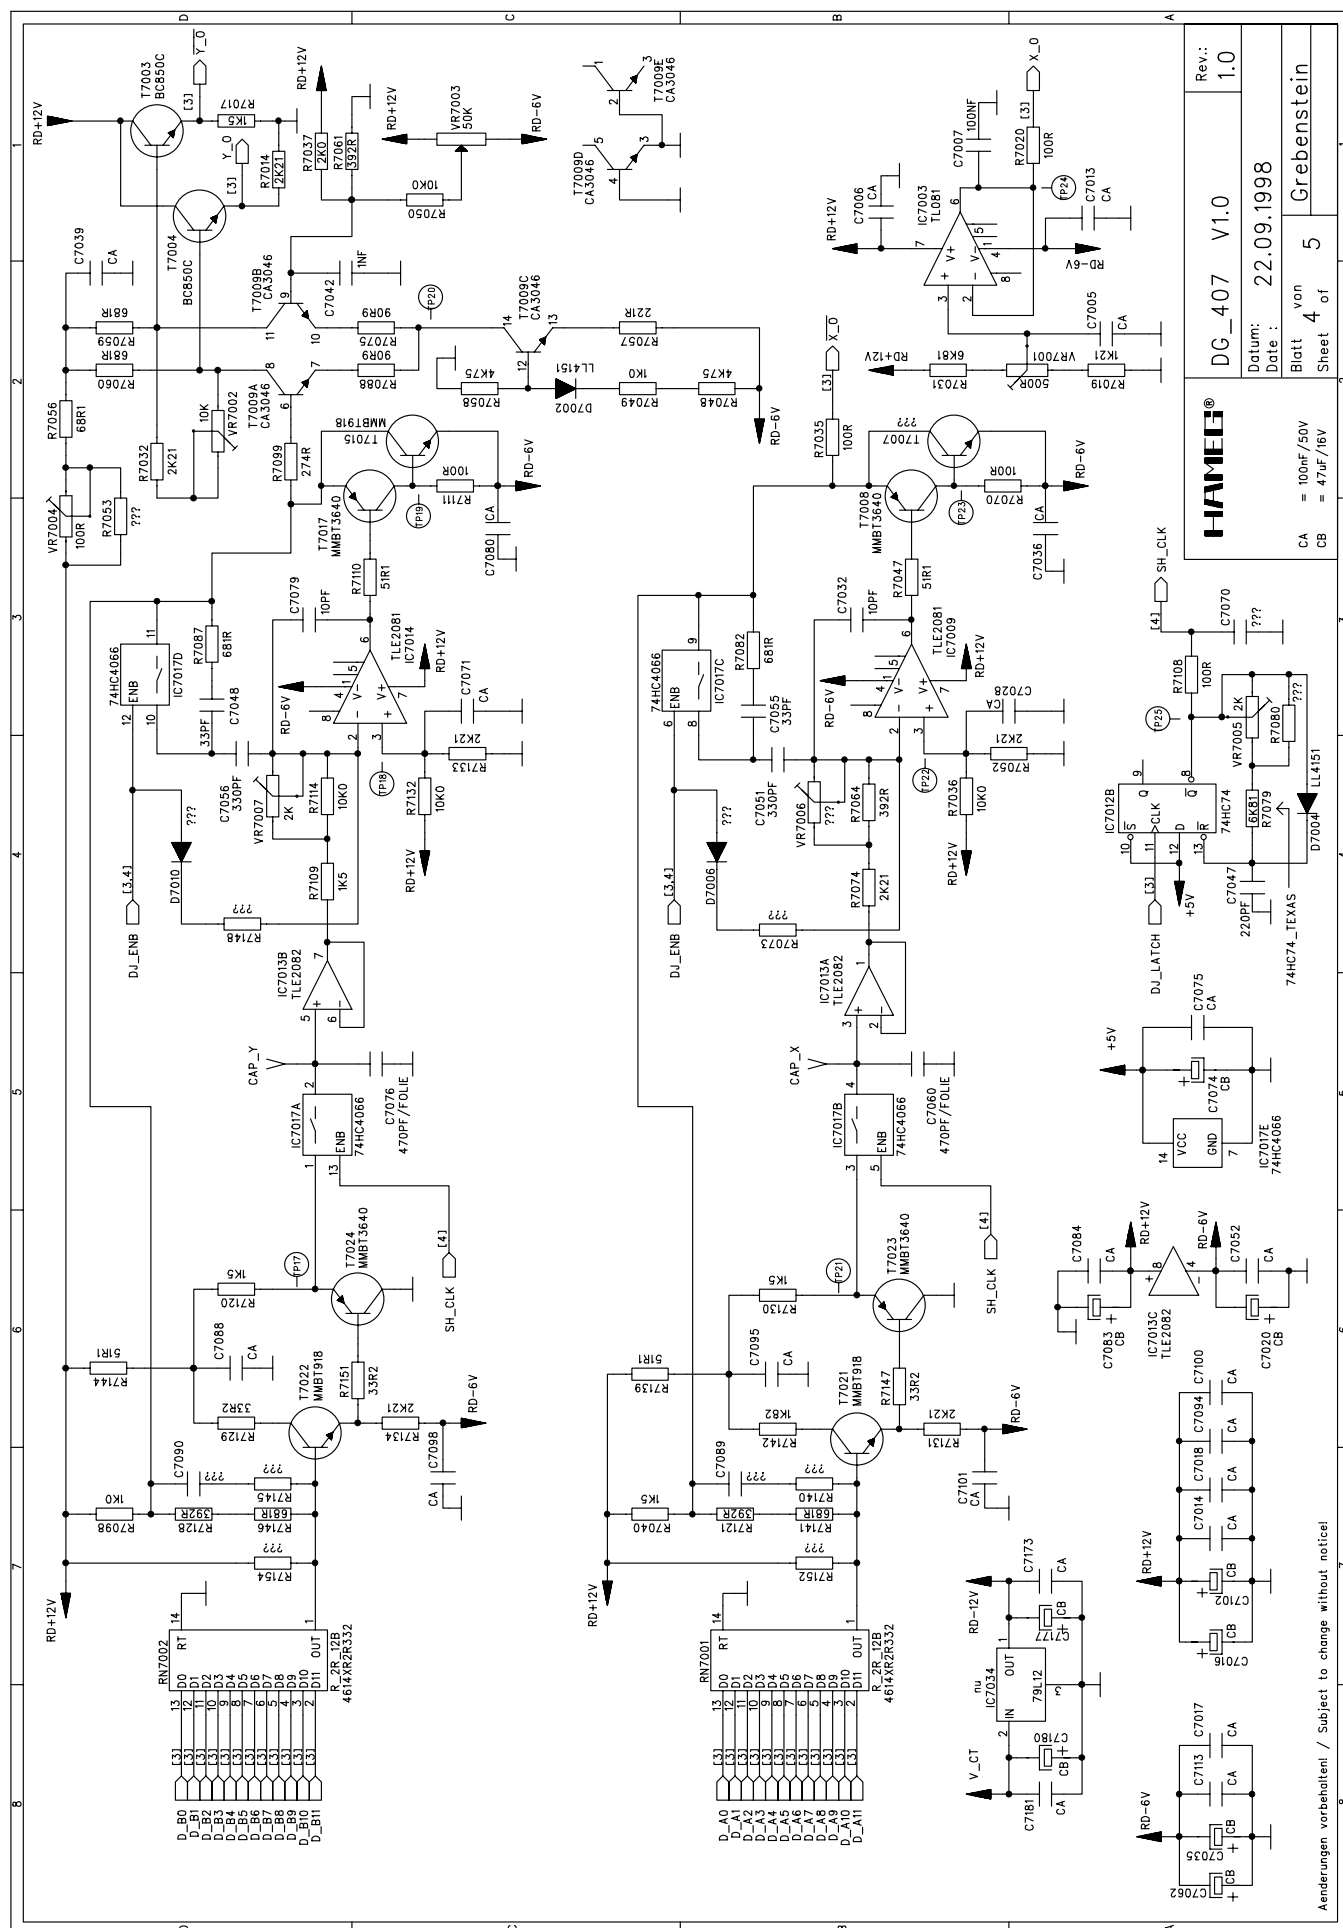


MT7001 980316

DG_407 V1.0


VP7001






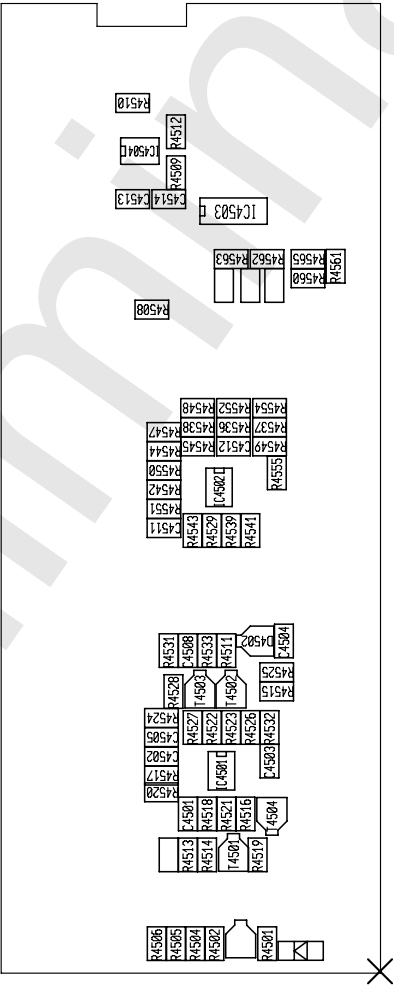


35-CCD0-0010 Rxx

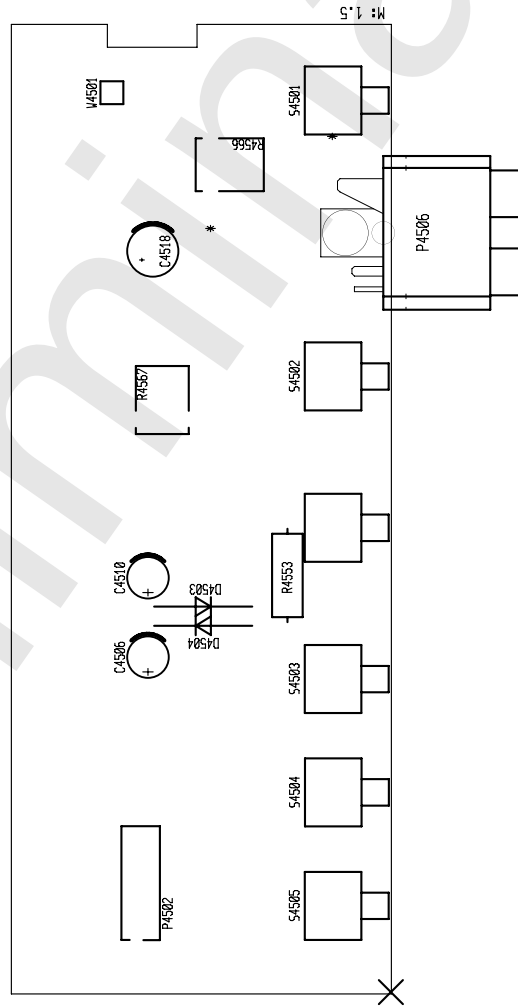


35-CCD0-0010 Rxx



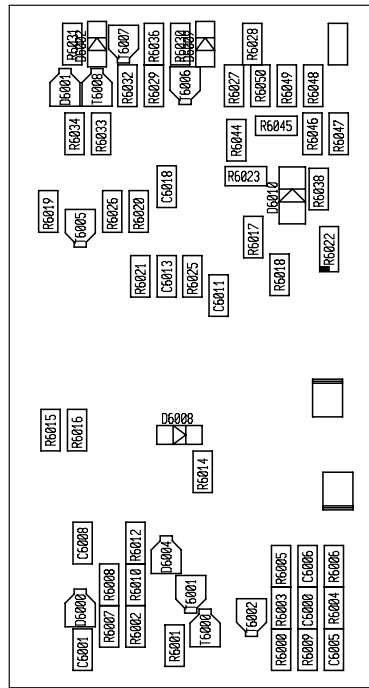


C6007 nicht bestückt !

CRT-NBV2.0R00

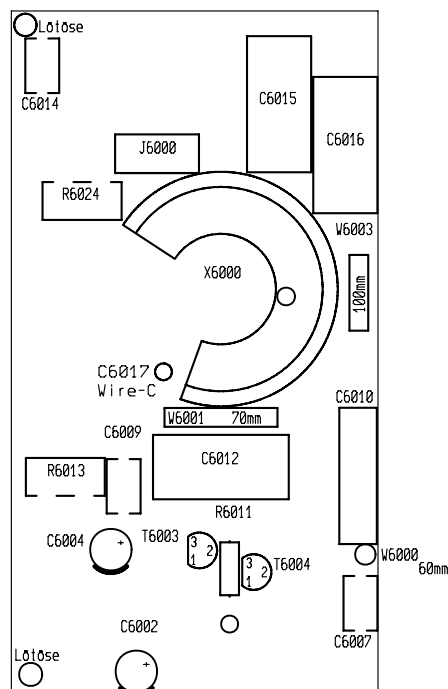



CRT-NBV2.0R00

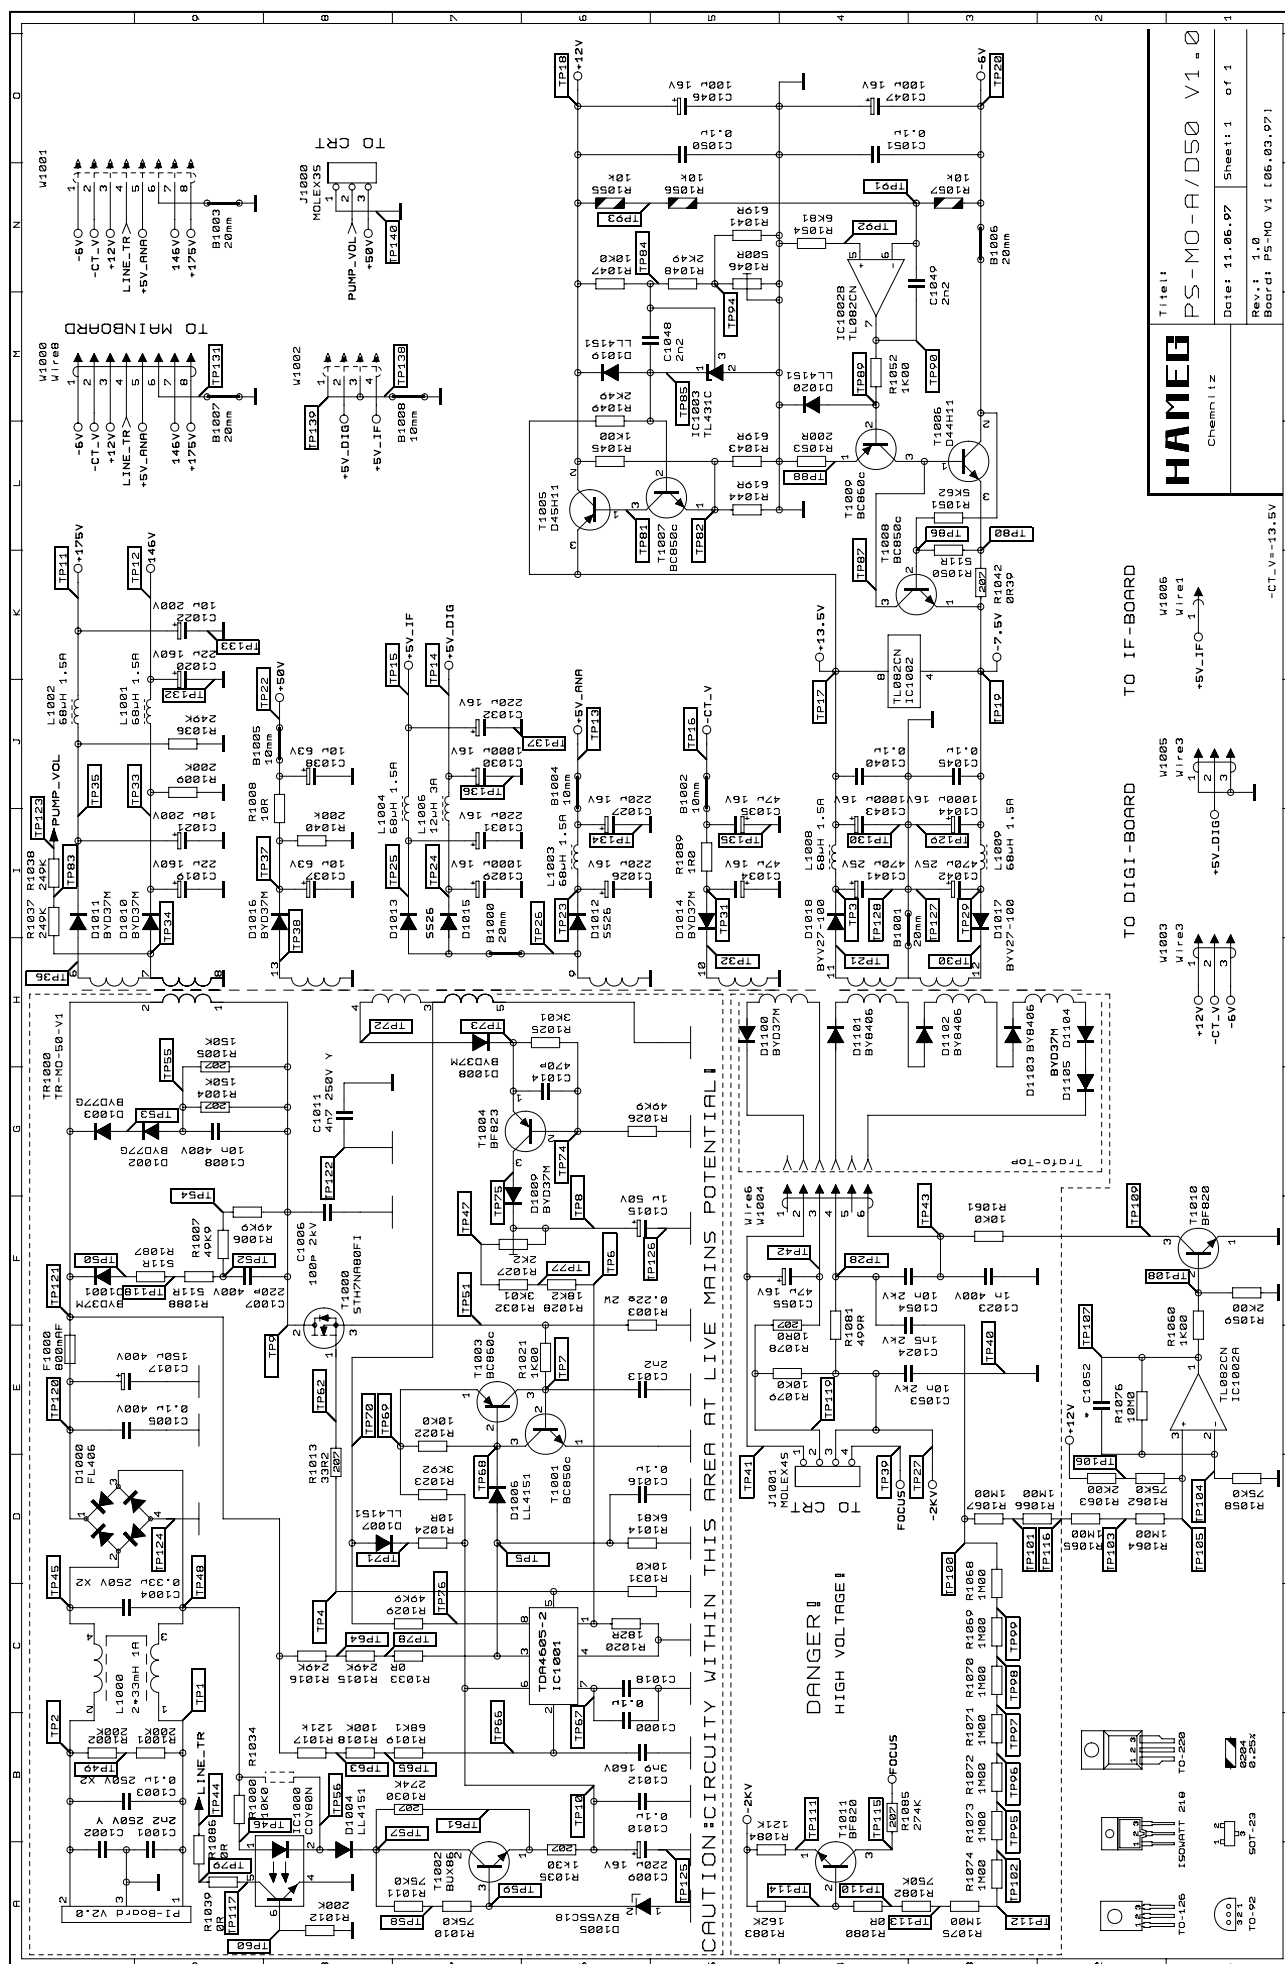




PS-MO-A40
Variante 1.0
28.10.97

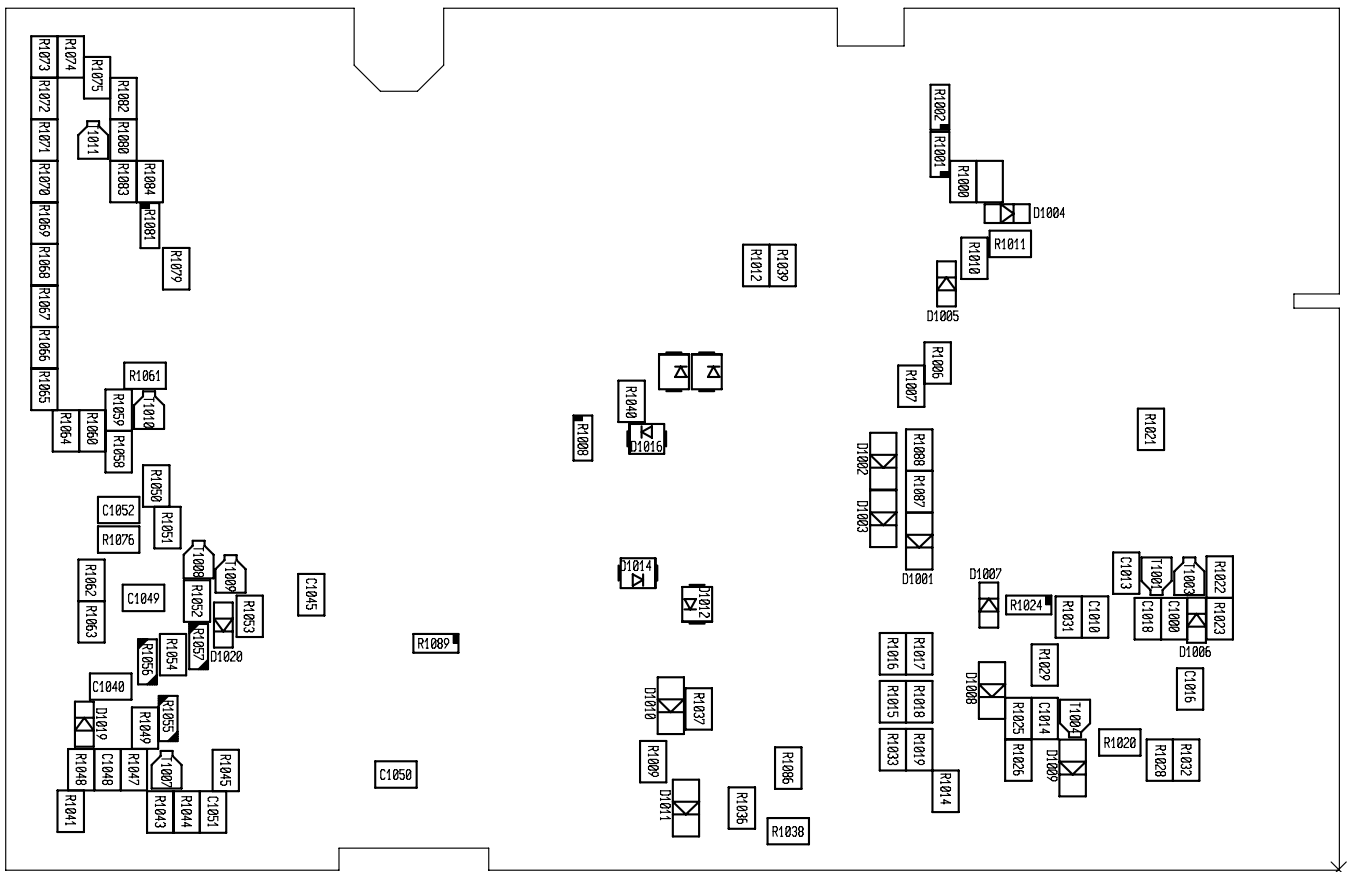

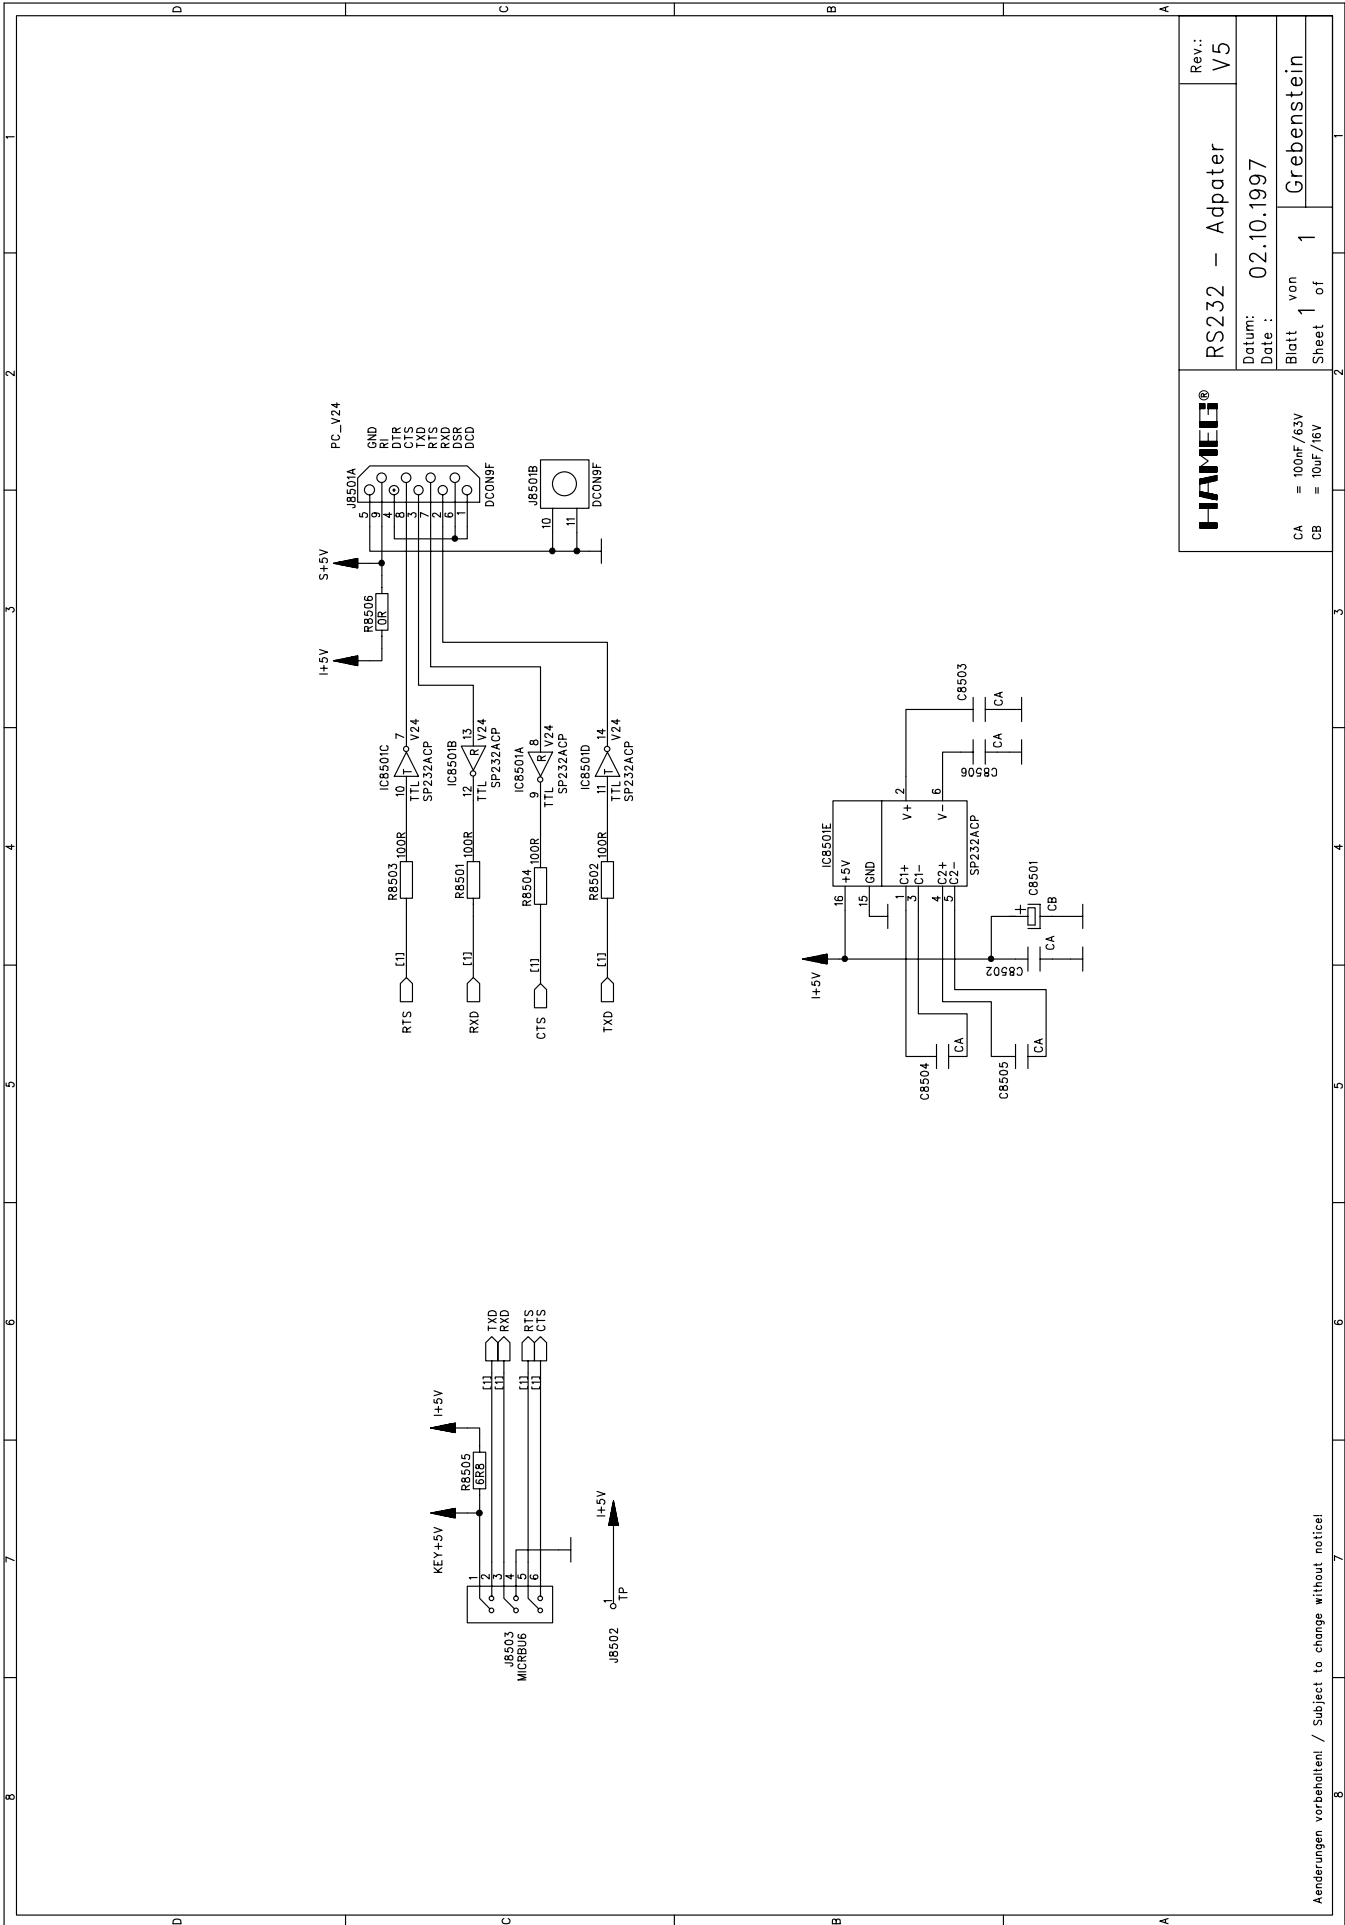

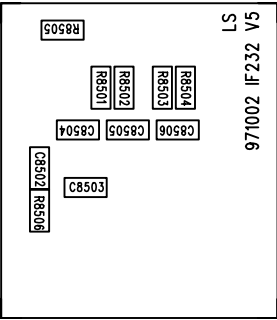

HAMEG[®]

Instruments

Oscilloscopes

Multimeters

Counters

Frequency Synthesizers

Generators

R- and LC-Meters

Spectrum Analyzers

Power Supplies

Curve Tracers

Time Standards

4S-0407-02E0

HAMEG GmbH

Industriestraße 6

63533 Mainhausen

Telefon: (0 61 82) 89 09-0

Telefax: (0 61 82) 89 09-30

E-mail: sales@hameg.de

Internet:

www.hameg.de

Printed in Germany