

TYPE 1208-C UNIT OSCILLATOR



This manual is provided FREE OF CHARGE from EBAMAN.COM as a service to the technical community.

It was uploaded by someone who wanted to help you repair and maintain your equipment.

If you paid for this manual, you paid someone who is making a profit from the free labor of others without asking their permission.

Thousands of files are available without charge from: EBAMAN.COM

Visit us at http://ebaman.com

This file was provided by: Jerry Ingordo W2JI

OPERATING INSTRUCTIONS

TYPE 1208-C UNIT OSCILLATOR

Form 1208-0100-1 March, 1966

Copyright 1963 by General Radio Company West Concord, Massachusetts, USA

GENERAL RADIO COMPANY
WEST CONCORD, MASSACHUSETTS, USA

TABLE OF CONTENTS

Section 1.	INTRODUCTION	Pa	age
	1.1 Purpose	•	1 3
	1.5 Auxiliary Equipment	•	3
Section 2.	OPERATING PROCEDURE		
	2.1 Installation		
Section 3.	APPLICATIONS		
	3.1 General	•	8 9
C 4.3 4	3.4 Unit Oscillator as a Frequency Converter	•	9
Section 4.	SERVICE AND MAINTENANCE		
	4.1 Warranty	•	10 10
•	4.2 Service	•	11
	4.4 Frequency Calibration	•	12

SPECIFICATIONS

Frequency Range: 65 to 500 Mc.

Tuned Circuit: Variable L and C with sliding contacts.

Frequency Calibration Accuracy: $\pm 2\%$. Warmup Frequency Drift (Typical): 0.5%.

Frequency Control: A six-inch dial with calibration over 250°, with a slow-

motion drive of about 10 1/2 turns.

Output Power into 50 Ohms with Type 1269-A (or 1203-B) Supplies:

240 mw from 65 to 250 Mc > 80 mw from 250 to 500 Mc

Output Power into 50 Ohms with Type 1201-B, 1264-A or 1267-A Supplies: 170 mw from 65 to 250 Mc > 60 mw from 250 to 500 Mc

Output System: A coupling loop at the rear of the instrument feeds a Type 874 locking coaxial connector through a short, rigid coaxial line. The coupling loop can be adjusted over a wide range to control power output, and can be clamped in any position.

Modulation: An external audio-frequency plate modulator can be connected to the front panel MODulation jack. The modulation impedance is approximately 8000 ohms. A sine wave of 40 volts rms amplitude will produce approximately 30% amplitude modulation. For 400- and 1000-cycle modulation, the Type 1214-A Unit Oscillator is recommended. For minimum incidental fm, a Type 1000-P6 Crystal Diode Modulator or a Type 1000-P7 Balanced Modulator can be connected between the rf output and the load.

Power Supply: Four types of power supply are recommended; refer to Table of Accessories, paragraph 1.5. The choice of power supply depends on the intended application.

Tube: One 2C43.

Mounting: L bracket with 7-inch-high panel for rigid attachment to companion power supply and easy relay-rack mounting.

Accessories Supplied: Type 874-R22LA Patch Cord, telephone plug.

Accessories Available: Refer to Table 1, paragraph 1.5.

Dimensions: Width 8, height 7 5/8, depth 8 1/2 inches (205 by 195 by 220 mm), over-all.

Net Weight: 6 pounds (2.8 kg).

U.S. Patent No. 2,548,457

General Radio Experimenter References: Vol 37 No. 8 August 1963

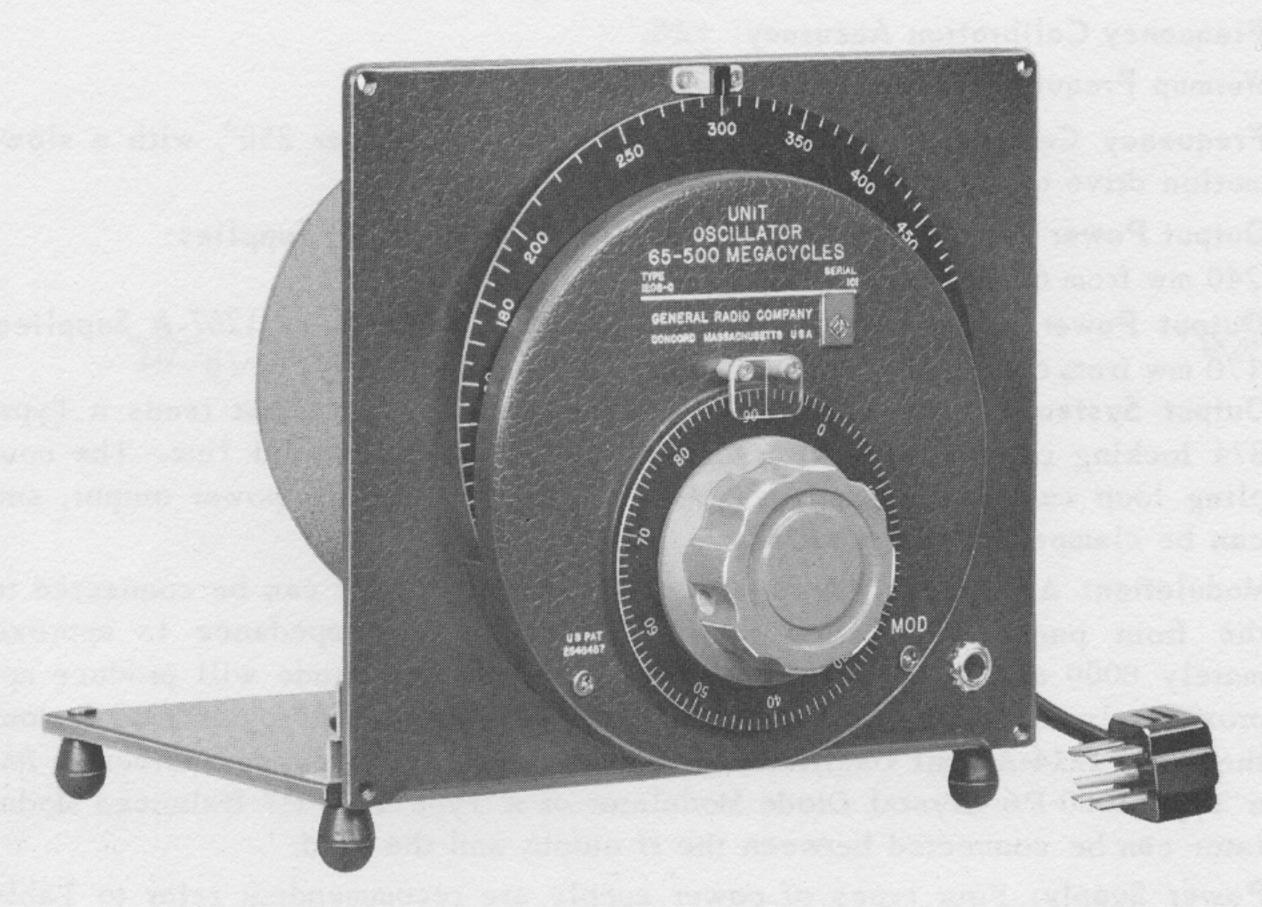


Figure 1-1. Panel view of the Type 1208-C Unit Oscillator.

SECTION

INTRODUCTION

1.1 PURPOSE.

The Type 1208-C Unit Oscillator (Figure 1-1) is a general-purpose power source for the radio-frequency laboratory. Covering the range from 65 to 500 Mc, this member of the convenient Unit Instrument line can be used to drive bridges, slotted lines, impedance comparators, and other measuring equipment. Used with a voltmeter and attenuator, it provides an accurately known output voltage for the testing of receivers. Direct amplitude modulation is possible over the audio-frequency range, and amplitude modulation free from incidental fm can be obtained with a simple crystal-diode modulator from zero to 5 Mc. Connected to a mixer, the Unit Oscillator can be used as the local oscillator in a heterodyne receiver to convert the Type 1216-A Unit I-F Amplifier or a low-frequency communications receiver into vhf or uhf detector. Pulsing and linear 100-percent amplitude modulation can be obtained with an external balanced modulator.

1.2 DESCRIPTION.

1.2.1 GENERAL. The tuning system of the Type 1208-C Unit Oscillator is a "contact-type" circuit, which combines a variable air capacitor and a variable inductor in a single unit. Inductance varies from 0.06 μh at the low-frequency end to 0.01 μh at the high-frequency end, and capacitance varies from 100 pf to 8 pf. Rotor and stator plates are shaped so that frequency varies logarithmically with dial rotation. The vernier dial requires about 10 1/2 turns to rotate the main dial over its full 250 degrees. The frequency calibration is accurate within 2 percent.



Plate and grid of the Type 2C43 lighthouse oscillator tube are connected to the tuned circuit, and the cathode shell is grounded. The oscillator circuit is of the Colpitts type, with feedback determined essentially by the electrode capacitances of the tube.

1.2.2 OUTPUT SYSTEM. The output system is a short coaxial line, with a coupling loop on one end and a Type 874 Coaxial Connector on the other. Coupling between the loop and the oscillator can be adjusted over a wide range, and the loop can be clamped in the desired position. Maximum power can be delivered to load impedances normally encountered in coaxial systems.

Power available into a 50-ohm load is plotted against frequency in Figure 1-3 for a typical Type 1208-C Unit Oscillator.

- 1.2.3 FREQUENCY STABILITY. For many applications a well-regulated and filtered power supply should be used to avoid frequency variations caused by line-voltage fluctuation and to produce a clearer beat note at the highest frequencies. With an unregulated power supply, a line-voltage variation of 20 percent causes a frequency change of about 0.01 percent at frequencies up to 300 Mc, 0.1 percent at 400 Mc, and 0.5 percent at the top end of the frequency range.
- 1.2.4 POWER REQUIREMENTS. The Type 1208-C Unit Oscillator requires an external power supply. The choice among the four General Radio power supplies recommended in paragraph 1.5 should be based on the intended application of the oscillator. If a power supply other than one of those recommended is used, it should be capable of delivering 300 to 320 volts dc at 40 ma for the plate and 6.3 volts at 0.9 ampere for the heater. The Type 1208-C Unit Oscillator cannot be used with the Type 1263-B Amplitude-Regulating Power Supply or with the Type 1264-A Modulating Power Supply because the cathode of the oscillator is grounded directly to the oscillator mounting bracket.


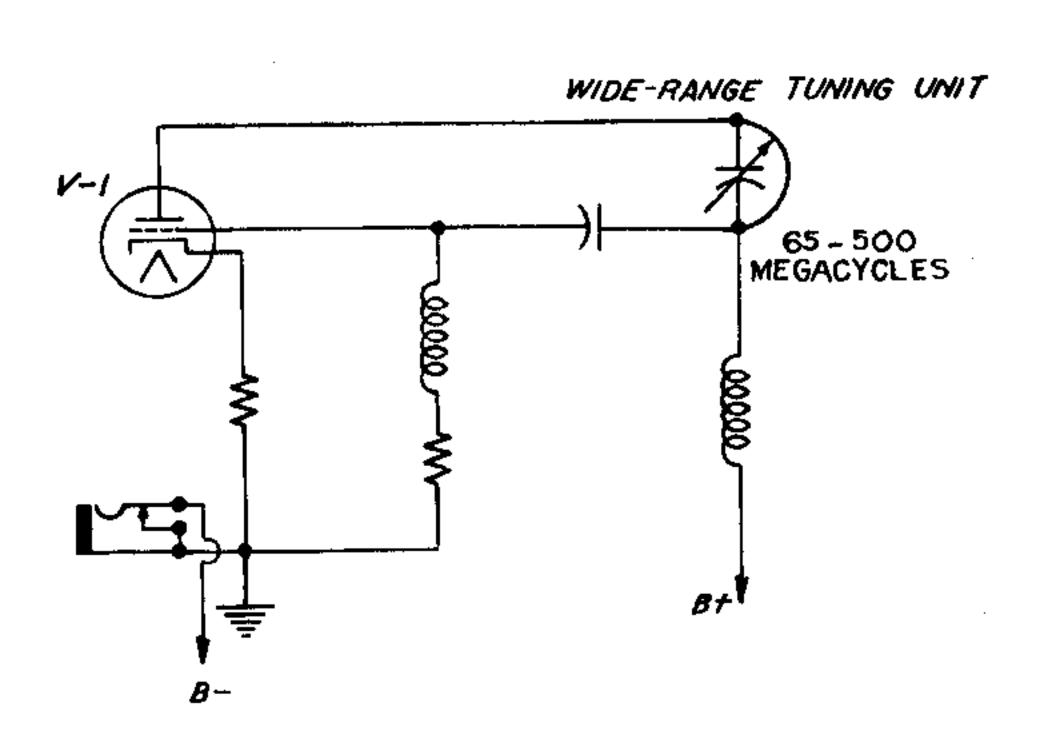


Figure 1-2. Elementary schematic diagram of the Type 1208-C Unit Oscillator.

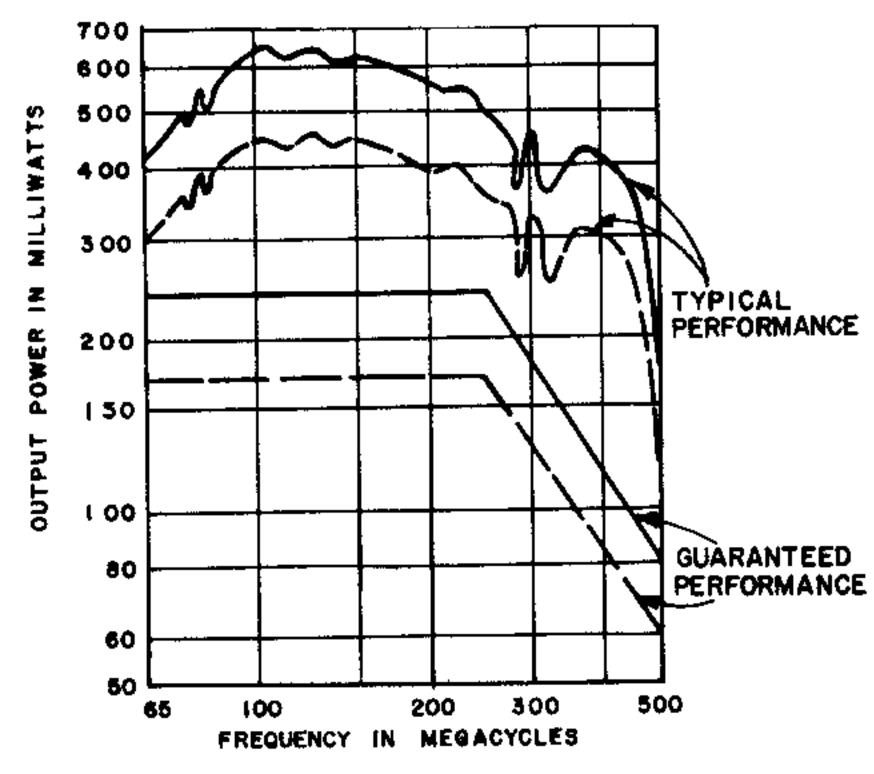

---WITH TYPE 1269(OR TYPE 1203) POWER SUPPLY

Figure 1-3. Output power into a 50-ohm load for a typical Type 1208-C.

1.2.5 ACCESSORIES SUPPLIED. Supplied with the Unit Oscillator are a Type 874-R22LA three-foot coaxial double-shielded Patch Cord and a phone plug.

1.3 AMPLITUDE MODULATION.

- 1.3.1 GENERAL. Amplitude modulation permits increased detection sensitivity through the use of a tuned amplifier, such as the General Radio Type 1232-A, following the rf detector. Recommended modulators are described in paragraph 1.5.
- 1.3.2 SINUSOIDAL AMPLITUDE MODULATION. A jack on the front panel of the oscillator permits connection of a plate modulator such as the Type 1214-A Oscillator. Appreciable incidental fm will accompany the amplitude modulation produced in this manner, especially at the high-frequency end of the tuning range. The audio oscillator must supply a dc path and must be able to carry 40 milliamperes dc. A sine wave of 40 volts rms amplitude will produce approximately 30% amplitude modulation.
- 1.3.3 ABSORPTION AMPLITUDE MODU LATION. Amplitude modulation free from incidental fm can be obtained by connection of a crystal-diode absorption modulator between the oscillator output and the equipment under test. With the Type 1000-P6 Crystal Diode Modulator, 30% amplitude modulation can be obtained with a peak output of 10 millivolts across 50 ohms. With the Type 1000-P7 Balanced Modulator, excellent pulse modulation with 60-db carrier suppression between pulses and 20-nanosecond rise time is possible. The peak rf output is 10 millivolts across 50 ohms.

1.4 SWEEP OPERATION.


For occasional use, the frequency dial of the Type 1208-C Unit Oscillator can be mechanically swept back and forth by a Type 908-P1 or 908-R96 Dial Drive, but this mode of operation is not recommended because neither the bearings nor the sliding contacts in the oscillator are designed for sweep use. Lubrication of all moving parts (described in paragraph 4.5) is particularly important if the oscillator is mechanically swept.

1.5 AUXILIARY EQUIPMENT.

The Type 1208-C Unit Oscillator can be used in conjunction with a variety of auxiliary General Radio equipment to build a signal source system which is suited to specific requirements. Typical systems are shown in Figure 1-4.

Table I lists the accessories recommended for use with the Type 1208-C Oscillator. The choice of a recommended power supplyor modulator should be based on the intended application of the oscillator. The Type 1267-A or 1269-A Power Supply can be readily attached to the Unit Oscillator to form a single unit for bench use or for relay-rack mounting with the listed adaptor plate set.



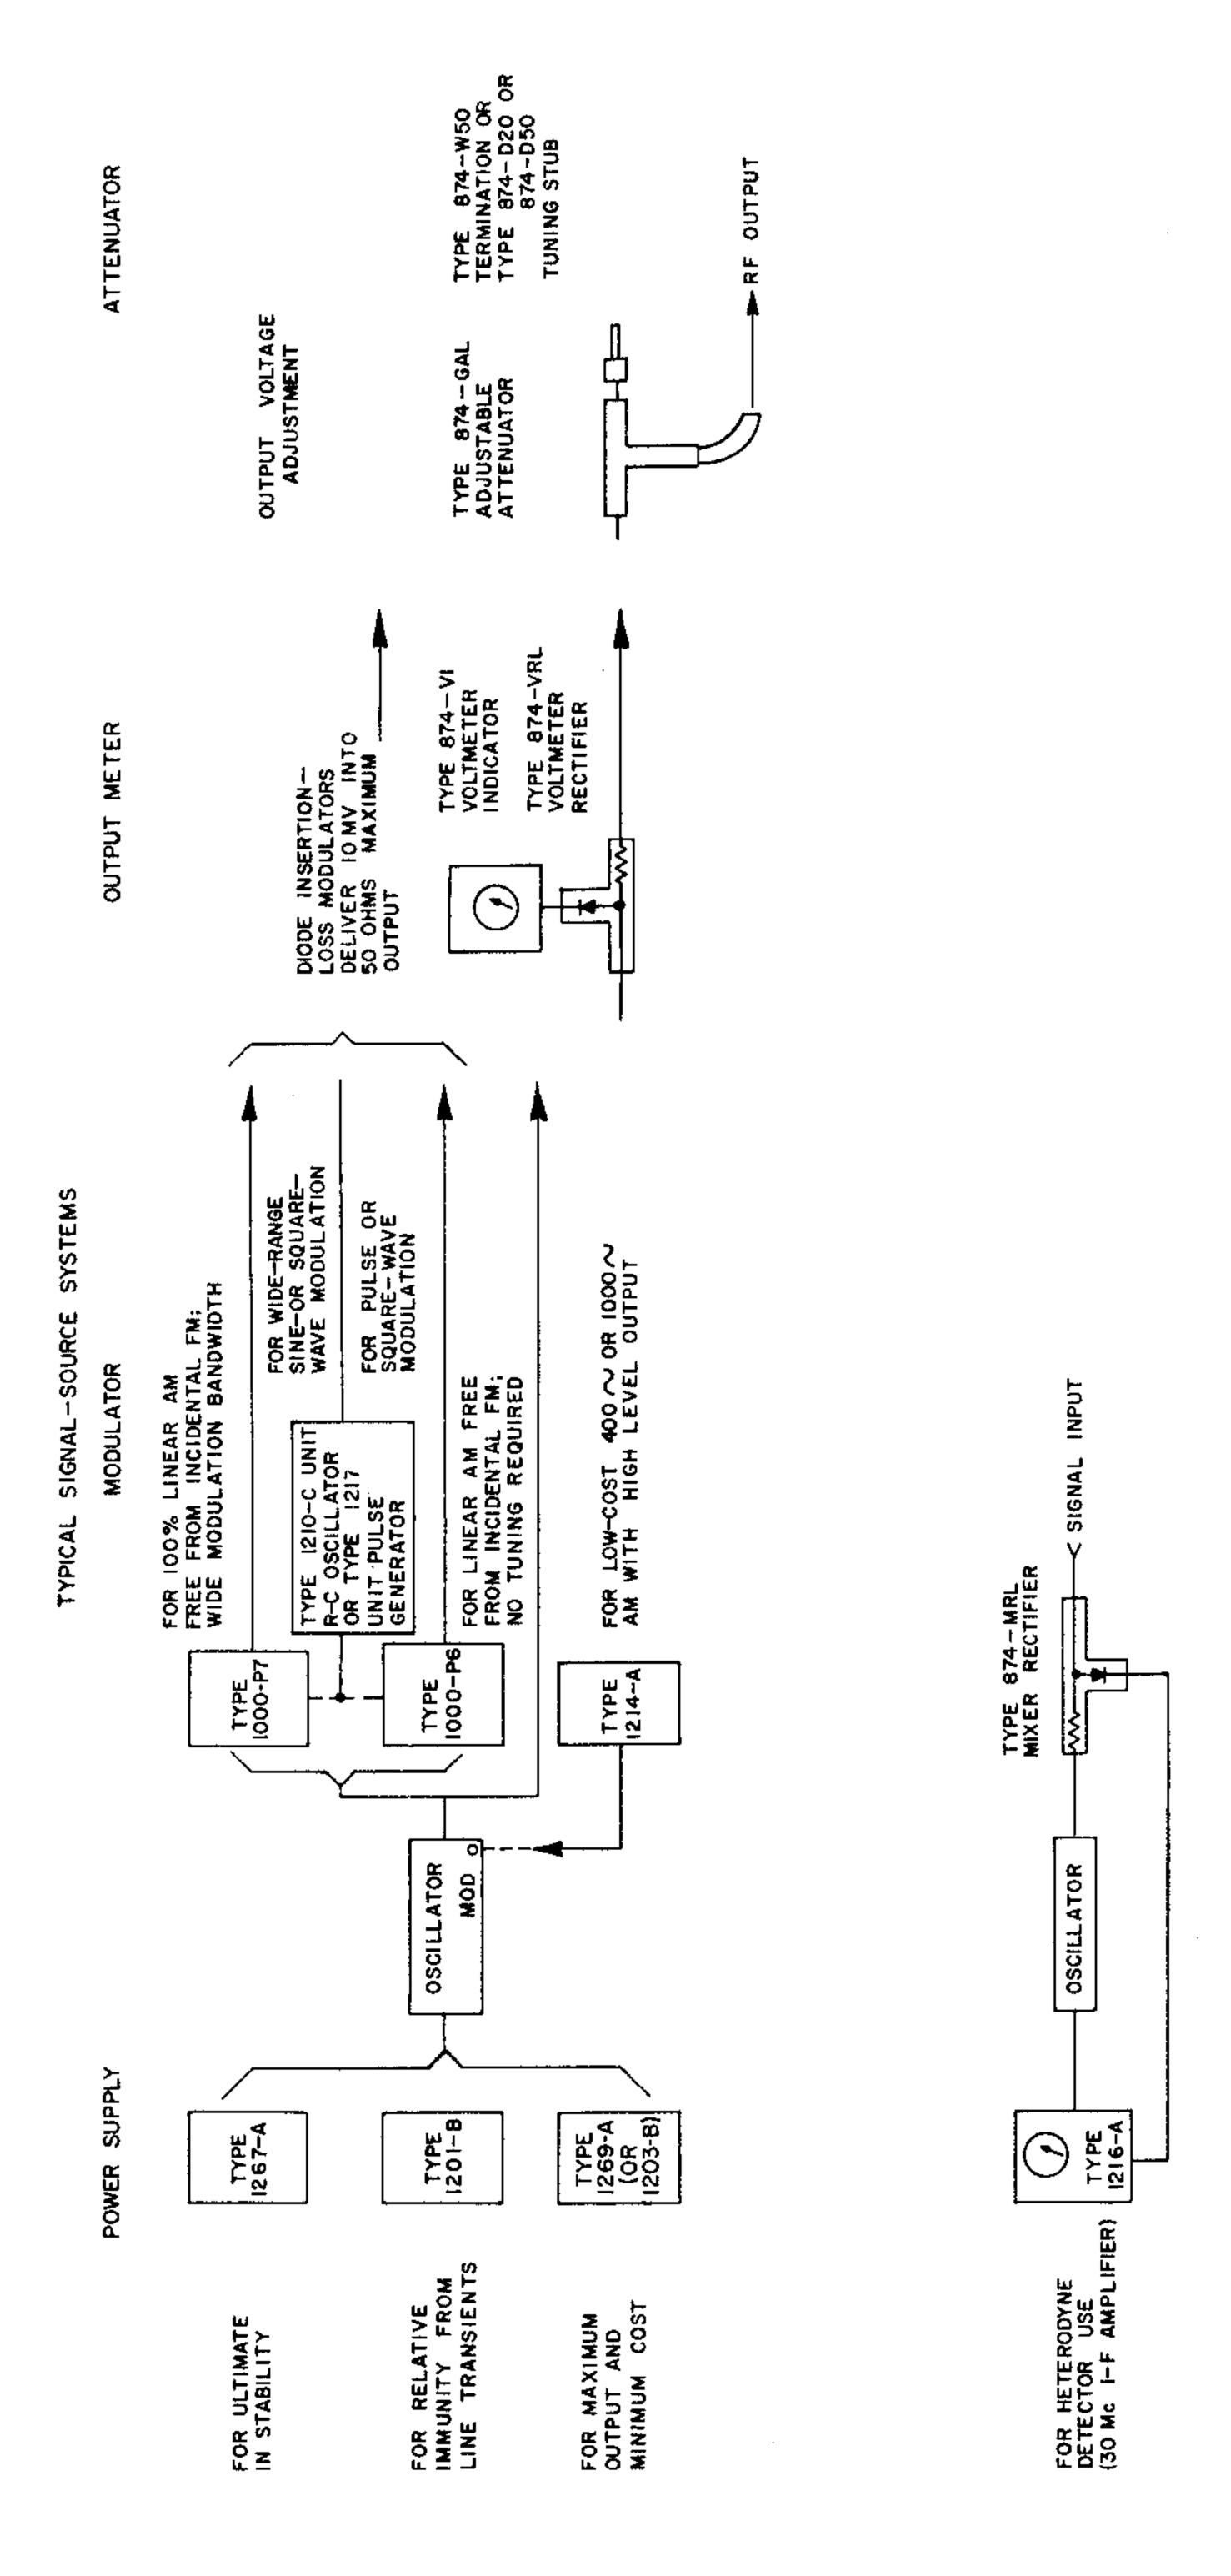

equipment associated and Oscillator Unit Ø with built systems source signal Typical Figure

TABLE 1 - ACCESSORIES

FUNCTION	INSTRUMENT	REMARKS
POWER SUPPLIES		
For best stability, freedom from line-voltage variations, and minimum residual fm.	Type 1267-A Power Supply	Regulated dc plate and heater supplies.
For relative immunity from line transients.	Type 1201 Unit Power Supply	Regulated dc plate supply and un- regulated ac heater supply.
For maximum output at minimum cost.	Type 1269-A (or 12-03-B) Power Supply	Filtered dc plate supply and ac heater supply, both unregulated.
For use as local oscil- lator in heterodyne de- tector system.	Type 1216-A Unit I-F Amplifier	30-Mc center-frequency amplifier has calibrated attenuator and output meter. Use with Type 874-MR Mixer Rectifier.
MODULATORS		
For sinusoidal plate modu- lation at 400 and 1000 cps.	1 -	Provides 30% modulation.
Absorption modulation with no incidental fm.	Type 1000-P6 Crys- tal Diode Modulator	30% modulation; 10 mv peak rf out- put into 50 ohms. Requires modu- lation source.
Pulse modulation with excellent carrier suppression. Absorption modulation with no incidental fm.	Type 1000-P7 Balanced Modulator	100% modulation; 10 mv peak rf output into 50 ohms; 20-Mc modulation bandwidth. Requires modulation source.
ADAPTOR PLATE SETS		
	Type 480-P408 Adaptor Plate Set	
To rack-mount the oscil- lator with a Type 1267-A or 1269-A Power Supply.	Type 481-P412 Adaptor Plate Set	
COAXIAL ELEMENTS S	ee table at the rear	of this manual.
To convert from Type 874 to other coaxial systems.	Type 874-Q Adaptors	
To reduce standing-wave ratio on transmission lines.	Type 874-G Attenuators	
To reduce harmonic content of output from oscil- lator.	, , –	
For use in a heterodyne detector system.	Type 874-MR (-MRL) Mixer Rectifier	Particulary useful with Type 1216-A Unit I-F Amplifier.
To provide monitored output level.	Type 874-VR (-VRL) Voltmeter Rectifier	Use with Type 874-VI Voltmeter Indicator.



SECTION 2

OPERATING PROCEDURE

2.1 INSTALLATION.

2.1.1 CONNECTION TO POWER SUPPLY. The Unit Oscillator is shipped complete with tube installed, and is ready for use when connected to a suitable power supply. A cord and connector are supplied with the instrument for direct connection to a General Radio Power Supply. Refer to paragraph 1.5 for power-supply recommendations.

To connect the oscillator to the power supply, plug the oscillator power cable into the receptacle on the side of the power supply.

- 2.1.2 BENCH MOUNTING. The Type 1267-A or Type 1269-A Power Supply can be rigidly attached to the oscillator by means of the attaching clips and associated screws supplied with the power supply and the clip which is attached to the oscillator L bracket with the mounting screw for the left front foot. To attach the units, proceed as follows:
- a. Temporarily remove the upper and lower right-hand corner panel screws from the front panel of the power supply. Replace the spacers behind the front panel of the power supply with the attaching clips supplied, so that one surface of the clip rests on the inner side of the end frame. Reinstall the panel screws through the clip.
- b. Remove the front and rear left feet from the oscillator. Install the clip, freed from the front-foot mounting screw on the top surface of the oscillator L bracket, in the left-rear-foot-mounting location. Note that the L-bracket hole in this location is tapped 10-32 to secure the mounting screw; use the clearance hole in the clip. Do not replace the feet.
- c. Attach the oscillator to the power supply, by means of the exposed clips attached to the supply, with the screws, lockwashers, and hex nuts supplied. Remove the case from the supply and attach the clip (tapped hole) at the left-hand rear of the oscillator, through the clearance hole in the right-hand side panel of the power supply. The necessary screws and nut are supplied with the power supply. Reinstall the case on the supply.

- 2.1.3 RELAY-RACK MOUNTING. To rack-mount the oscillator by itself, a Type 480-P408 Adaptor Plate Set is required. To rack mount the oscillator attached to a Type 1267-A or 1269-A Power Supply, a Type 481-P412 Adaptor Plate Set is required. For either mounting, one plate is installed at the left-hand side of the unit and one at the right-hand side. The necessary screws are supplied with the Adaptor Plate Set. The procedure for installation is similiar to that described in paragraph 2.1.2.
- 2.1.4 RF OUTPUT CONNECTIONS. Connect the oscillator to the equipment under test by means of the three-foot coaxial cable supplied. If cables with military connectors are used, a suitable adaptor may be semipermanently attached to the locking Type 874 output receptacle of the oscillator. Refer to the table at the rear of this manual for a listing of the available adaptors.

Attenuator pads may help to reduce the standing waves on the cable where the equipment under test does not provide a good termination. Without padding, cable resonance effects may be quite pronounced since the output coupling loop of the oscillator is not a matched source. A low-pass filter may be beneficial in cases where oscillator harmonics must be kept to very low values.

2.1.5 MODULATOR CONNECTION. For amplitude modulation the audio modulating voltage should be inserted at the MODulation jack on the front panel. Full plate current must flow through the modulating source. A modulation voltage of about 40 volts is required for 30-percent modulation. The input impedance is about 8000 ohms. The Type 1214-A Unit Oscillator is an economical 400- and 1000-cycle modulator for the Type 1208-C Unit Oscillator.

2.2 OPERATION.

After turning on the power supply, adjust the frequency by means of the frequency dial, and adjust for maximum output by rotating the output coupling loop. To reduce the output, the coupling loop can be partly withdrawn. A setting of the coupling loop which is optimum at one frequency may not necessarily be desirable at another frequency, particularly if the load does not provide a good termination for the transmission line which connects it to the oscillator. If adequate padding (refer to paragraph 2.1.4) is used, a loop setting which is satisfactory at the high-frequency end of the tuning range will generally be suitable over the entire range.



SECTION 3

APPLICATIONS

3.1 GENERAL.

The utility and versatility of the Type 1208-C Unit Oscillator are greatly increased by the large selection of Type 874 coaxial elements available from General Radio Company. These elements are part of a complete, integrated line of equipment for the measurement of voltage, power, and standingwave ratio at very-high and ultra-high frequencies. Although the Unit Oscillator is intended primarily as a source of power for this measuring equipment and for other impedance measuring devices such as the Type 1602 UHF Admittance Meter, use of the coaxial elements can adapt the Unit Oscillator to various applications in the radio-frequency laboratory.

Three applications are described in detail in the following paragraphs. Others will be suggested by a study of the complete list of Type 874 coaxial elements included in the General Radio Catalog. Coaxial elements with either locking or nonlocking connectors can be used. A condensed list of Type 874 elements appears in the rear of this manual.

3.2 UNIT OSCILLATOR AS SIGNAL GENERATOR FOR RECEIVER TESTING.

The Type 1208-C, as a well-shielded power source, can be used as a signal generator to test receivers if means are available to measure and attenuate the output. The Type 874-VR Voltmeter Rectifier, Type 874-VI Voltmeter Indicator, and Type 874-GAL Adjustable Attenuator are suitable for this purpose, and should be connected to the Unit Oscillator as shown in Figure 3.1. Also, a Type 874-D50L Adjustable Stub is required at the higher frequencies (from 300 Mc up) to produce a current maximum at that point of the attenuator where the adjustable output loop is coupled. At lower frequencies

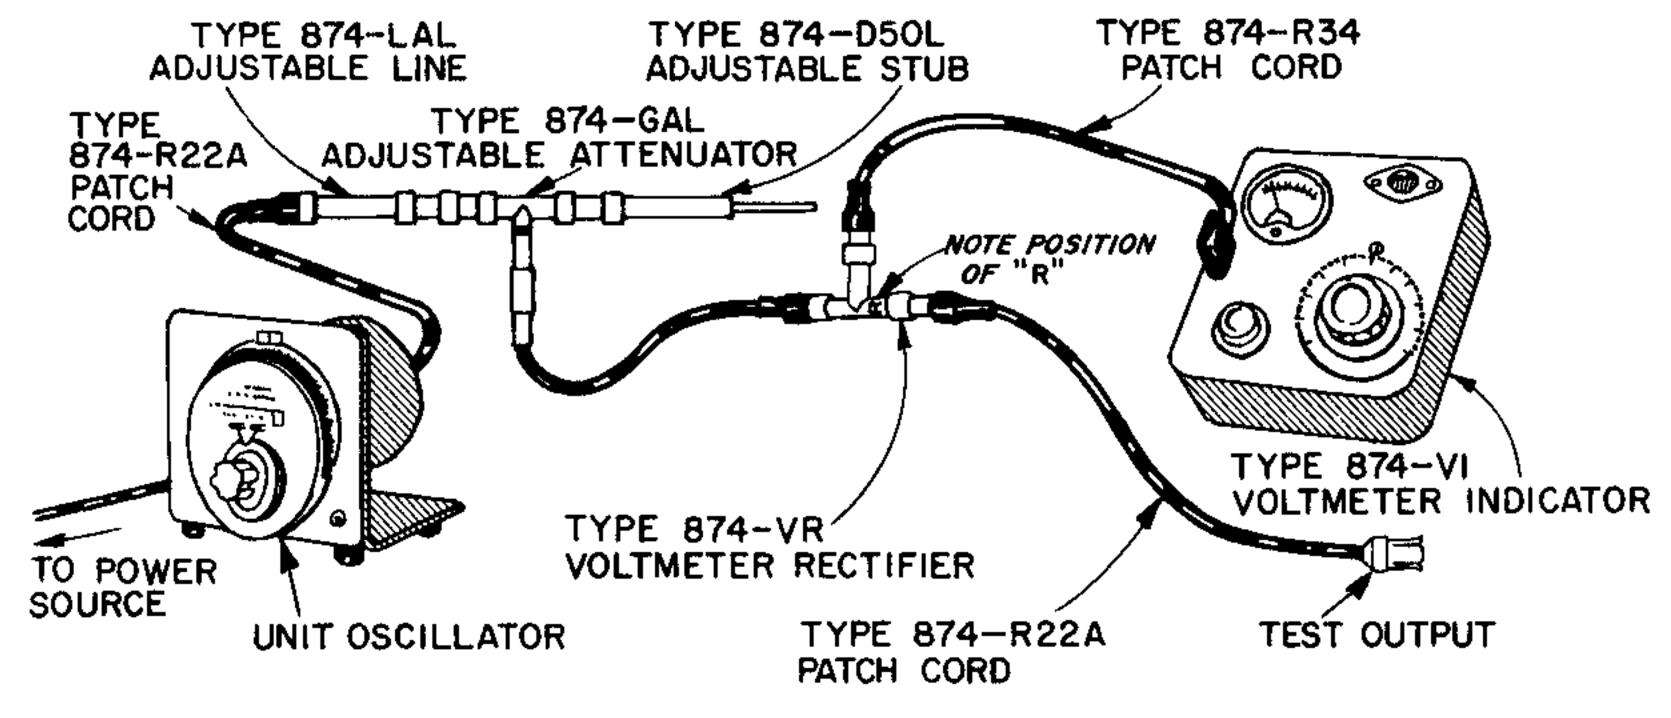


Figure 3-1. Unit Oscillator, with accessories, set up as a standard-signal generator.

a Type 874-WN Short-Circuit Termination can be used for this purpose. A tuning element between the oscillator and the attenuator is required to increase the output to a value that can be read on the voltmeter. At higher frequencies coverage is obtained by a Type 874-LAL Adjustable Line. At lower frequencies additional lengths of line must be used.

Current from the Unit Oscillator is fed through the attenuator into the short circuit or the stub. The attenuator is calibrated in decibels. At minimum attenuation the attenuator output is measured by a crystal diode in the voltmeter rectifier and read on the meter of the voltmeter indicator. Means are provided to standardize the crystal indication. A 50-ohm resistor after the crystal determines the output impedance.

With the above-described arrangement, the maximum available output is several tenths of a volt. The attenuator calibration covers 120 db, but shielding of the Unit Oscillator and of other components is not sufficient for accurate measurements in the microvolt region.

3.3 UNIT OSCILLATOR AS A TELEVISION-SIGNAL GENERATOR.

Used in combination with a Type 1000-P6 Crystal Diode Modulator and a Type 874-G20, 20-db Fixed Attenuator, the Unit Oscillator is a convenient source of television signals over its entire carrier-frequency range if video modulating voltage is available. (See Figure 3-2.) The modulating voltage required can be obtained from a standard television receiver tuned to a local channel. Since the modulator and oscillator are separated from each other by an attenuator pad, amplitude modulation is free from incidental fm. Output is about 10 millivolts.

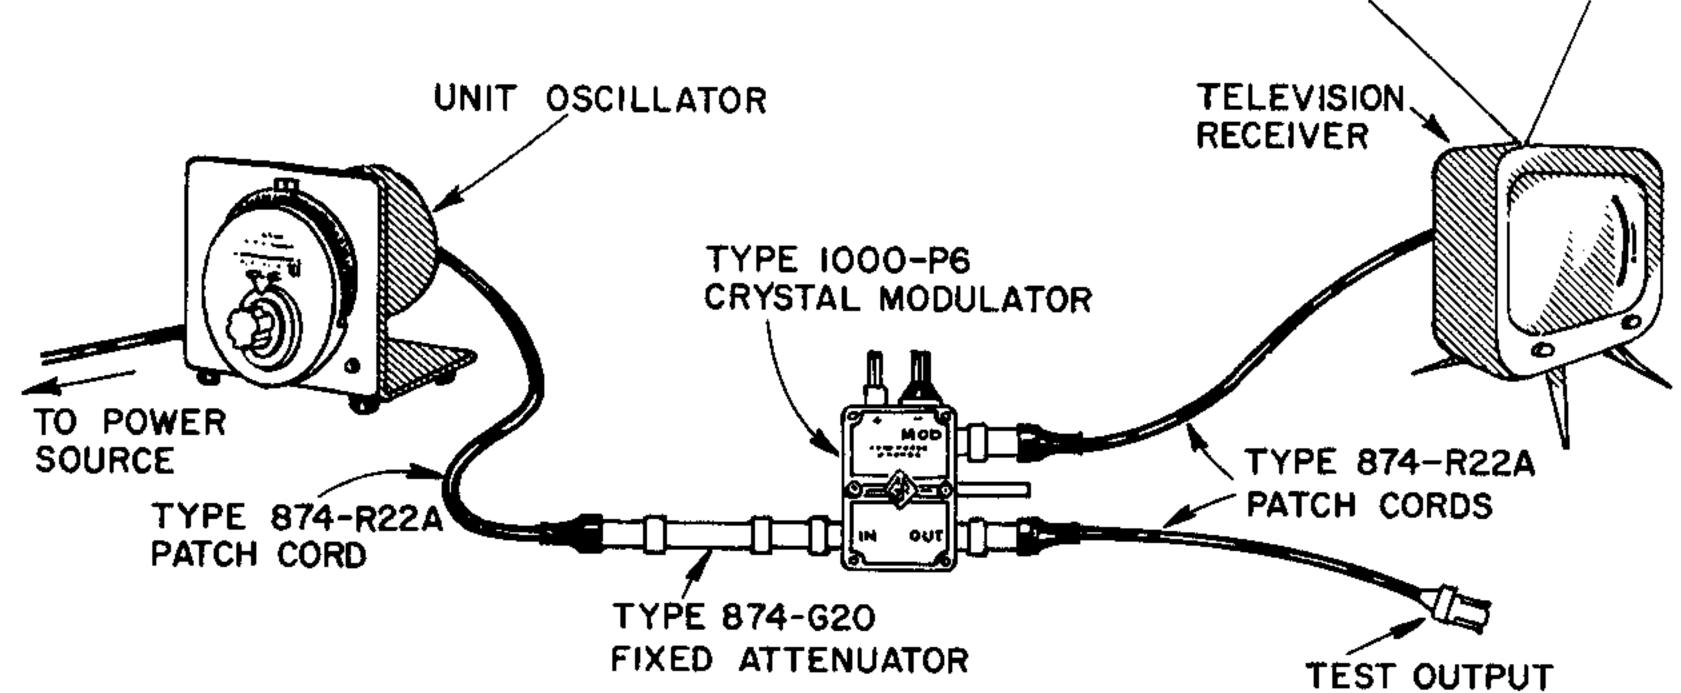



Figure 3-2. Setup of a Unit Oscillator with a video modulator for use as a television-signal generator.

3.4 UNIT OSCILLATOR AS A FREQUENCY CONVERTER.

Connected to a Type 874-MR Mixer Rectifier, the Unit Oscillator can provide the local signal in a heterodyne converter to adapt the Type 1216-A Unit I-F Amplifier for use as a sensitive detector for vhf and uhf signals. (See Figure 3-3.) Without additional tuning, the conversion loss is about 6 db at an intermediate frequency of 30 Mc.



Figure 3-3. Unit Oscillator, with mixer rectifier, set up as a frequency converter.

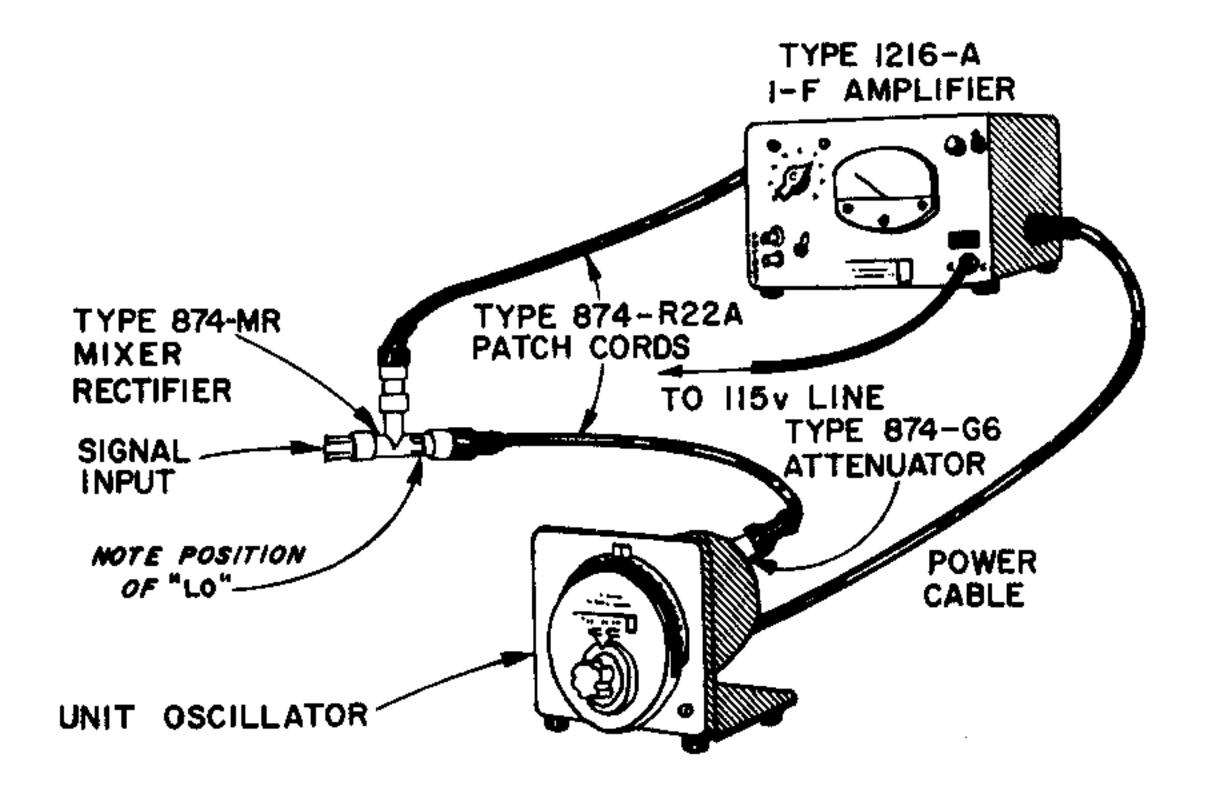

Similiar oscillators for other tuning ranges in the vhf-uhf region are as follows:

50 - 250 Mc Type 1215 250 - 960 Mc Type 1209-C 180 - 600 Mc Type 1209-CL 450 - 1050 Mc Type 1361 900 - 2000 Mc Type 1218

SECTION 4

SERVICE AND MAINTENANCE

4.1 WARRANTY.

We warrant that each new instrument sold by us is free from defects in material and workmanship, and that, properly used, it will perform in full accordance with applicable specifications for a period of two years after original shipment. Any instrument or component that is found within the two-year period not to meet these standards after examination by our factory, district office, or authorized repair agency personnel, will be repaired or, at our option, replaced without charge, except for tubes or batteries that have given normal service.

4.2 SERVICE.

The two-year warranty stated above attests the quality of materials and workmanship in our products. When difficulties do occur, our service engineers will assist in any way possible. If the difficulty cannot be eliminated by use of the following service instructions, please write or phone our Service Department (see rear cover), giving full information of the trouble and of steps taken to remedy it. Be sure to mention the serial and type numbers of the instrument.

Before returning an instrument to General Radio for service, please write to our Service Department or nearest district office (see back cover), requesting a Returned Material Tag. Use of this tag will ensure proper handling and identification. For instruments not covered by the warranty, a purchase order should be forwarded to avoid unnecessary delay.

4.3 TUBE REPLACEMENT.

If the oscillator tube is replaced, readjustment of the variable grid resistor and the series plate resistors may be required to obtain maximum output and to prevent overloading of the oscillator tube. The grid resistor, on the oscillator base casting, is accessible when the shield is removed. (To remove the shield, loosen the clamp screw and remove the two screws near the top of the shield.) The series plate resistors are inside the base casting, and their terminals project through the side of the base. The three terminals may or may not be shorted, depending on the characteristics of the oscillator tube. (See Figure 4-1.) When the shield is replaced, be sure to tighten the two screws near the top of the shield securely.

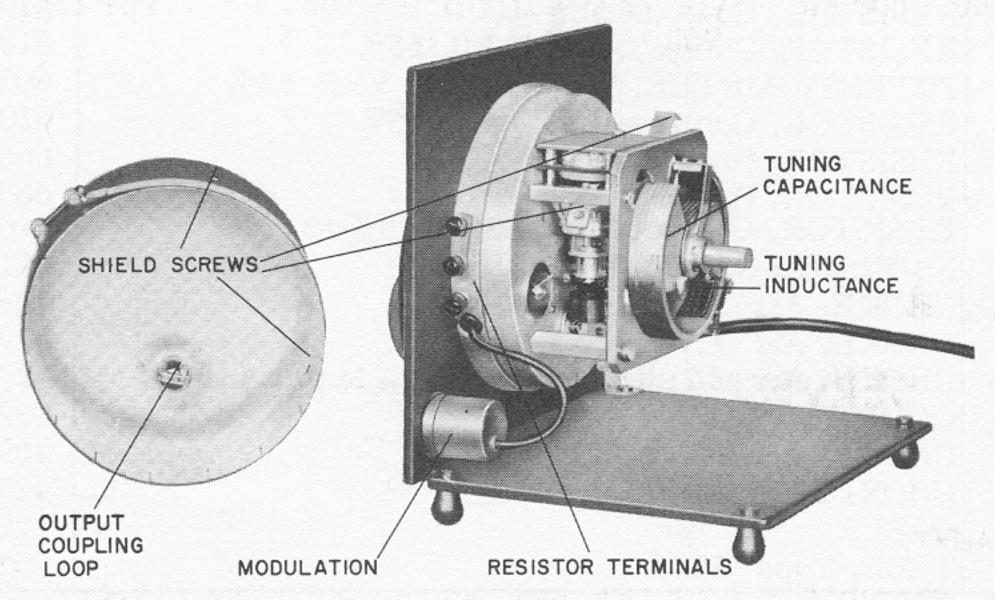


Figure 4-1. Unit Oscillator, with cover removed, showing the tuned circuit and output coupling loop (in cover).

The maximum allowable plate current is 36 milliamperes, and the maximum plate dissipation is 10 watts. For maximum output, the tube should operate near maximum plate current. Plate current is adjusted by means of the grid resistor R3. It will be found that maximum plate current is obtained under no load near the top end of the frequency range. With a fixed power supply with an output voltage over 275 volts at 36 milliamperes, plate series resistance (2000, 3500, or 5500 ohms) may be required to limit plate dissipation or to allow operation with a lower grid resistor R3 to prevent motor-boating.

4.4 FREQUENCY CALIBRATION.

Replacement of the oscillator tube may also affect frequency calibration. It can be restored by adjustment of the flexible tab on the plate connector. Before adjusting this trimmer capacitor, allow the instrument to warm up, since warm-up drift may be as much as 0.5 percent. This adjust-



ment should be carried out at the high-frequency end of the oscillator tuning range. It is also important to note that the oscillator shield affects frequency considerably, especially at the low-frequency end.

4.5 CLEANING AND LUBRICATION.

If, after some time, frequency can no longer be adjusted smoothly, clean the spring fingers and the contact surfaces on rotor and stator with carbon tetrachloride, and apply a thin film of light lubrication (Anderol x-2041-1A).

PARTS LIST

REF. NO.	DESCRIPTION	PART NO.
R1	RESISTOR, Composition 100Ω ±5%	6100-1105
R2	RESISTOR, Composition 1 k Ω ±5%	6100-2105
R3	POTENTIOMETER, Wire-wound 5 kΩ ±5%	6050-1700
R4	RESISTOR, Composition 1 k Ω ±5%	6100-2105
R 5	RESISTOR, Power $2 k\Omega \pm 5\%$	6650-2205
R 6	RESISTOR, Power 3.5 k Ω ±10% RESISTOR, Composition 22 Ω ±10%	6630-2359
R 7		6100-0225
J1	SHIELDED CABLE SET	1211-0300
L1	CHOKE, Air 1.75 μh	4290-0700
L2	CHOKE, Air 1.75 µh	4290-0700
L3	CHOKE, Air 45 μh	4290-0600
L4	COUPLING LOOP	0874-4010
L5	CHOKE, Air 92 μh	4290-1300
L6	CHOKE, Air 45 μh	4290-0600
PL1	CABLE	1208-0370
V1	TUBE, Type 2C43	8320-0200

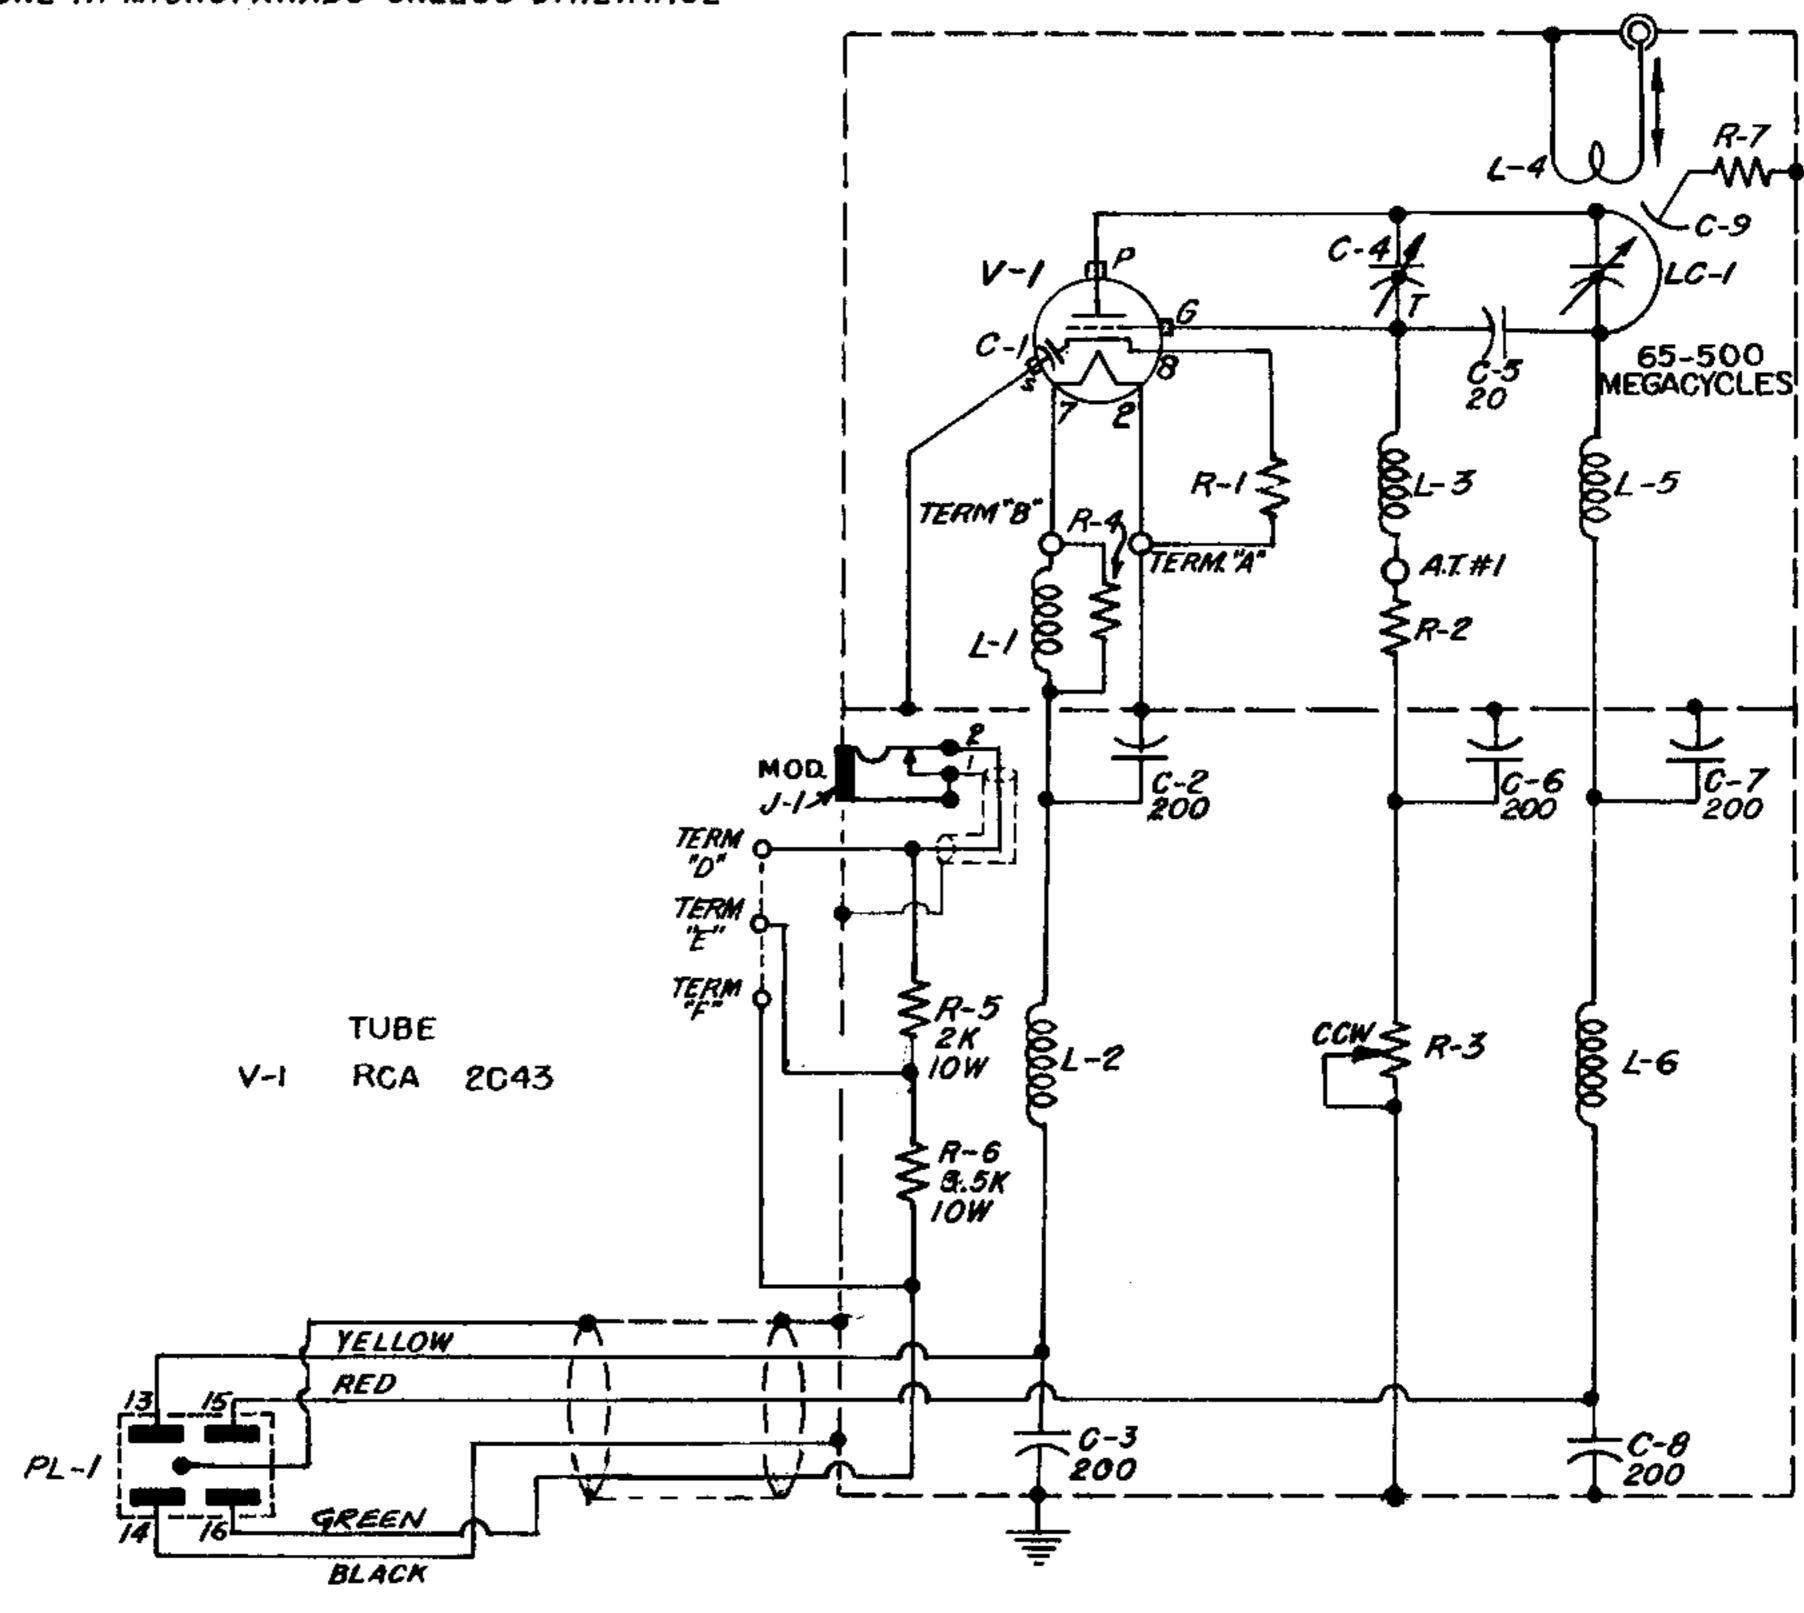


Figure 4-2. Schematic diagram for the Type 1208-C Unit Oscillator.

		TYPE 874 CABLE CONNECTORS				
	CONNECTOR	CABLE	CABLE LOCKING	PANEL FLANGED	PANEL LOCKING	PANEL LOCKING RECESSED
	874-A2	-CA	-CLA	-PBA	-PLA	-PRLA
50.0HM	RG-8A/U RG-9B/U RG-10A/U RG-87A/U RG-116/U RG-156/U RG-165/U RG-213/U RG-214/U RG-215/U RG-225/U RG-227/U	-C8A	-CL8A	- PB8 A	-PL8A	-PRL8A
CABLE TYPES	RG-11A/U RG-12A/U RG-13A/U					
APPLICABLE	874-A3 RG-29/U RG-55/U (Series)	-C58A	-CL58A	- PB58A	-PL58A	-PRL58A
MHC 63 NOW	PC-50 /11	-C62A	-CL62A	- PB62A	-PL62A	-PRL62A
NON	RG-174/U RG-188/U RG-316/U RG-161/U RG-187/U RG-179/U	-C174A	-CL174A	-PB174A	-PL174A	-PRL174A

TYPE 874 ADAPTORS TO TYPE 874-		
10	1 1 F E	874-
BNC	plug	QBJA QBJL* QBPA
	jack	
С	plug	QCJA QCJL*
	jack	QCP
HN	pług j a ck	QHJA QH P A
LC	plug	QLJA QLPA
LT	plug jack	QLT J QL P T
16:		QMDJ
Microdot	plug	QMDJL*
	jack	QMDP
N	plug	QNJA ONIL*
	jack	QNJL* QNP QNPL*
OSM/BRM	plug	QMMJ QMMJL*
	jack	QMMP QMMPL
SC (Sandia)	plug	QSCJL*
(~~~~	jack	QSCP
TNC	plug	QTNJ QTNJL*
	jack	QTNP
UHF	plug	QUJ QUJL*
	jack	QUP
UHF	7/8-in.	QU1A
50-Ω	1-5/8-in.	QU2
Air Line	3-1/8-in.	QU3A

*Locking Type 874 Connector

Example: To connect Type 874 to
a type N jack, order Type 874-QNP.

CONNECTOR ASSEMBLY TOOLS

TYPE 874- FUNCTION

TOK Tool Kit
TO58 Crimping Tool
Crimping Tool
Crimping Tool

OTHER COAXIAL ELEMENTS			
TYPE 874-		TYPE 874-	
A2 A3 D20L, D50L EL, EL-L F185L F500L F1000L F2000L F4000L F8L G3, G3L, G6, G61 G10, G10L G20, G20L GAL JR K, KL L10, L10L L20, L20L L30, L30L LAL LK10L, LK20L LR LTL	50 Ω cable (low loss) 50 Ω cable 20-, 50-cm adjustable stubs 90° ell 185-Mc/s low-pass filter 500-Mc/s low-pass filter 1000-Mc/s low-pass filter 2000-Mc/s low-pass filter 4000-Mc/s low-pass filter 4000-Mc/s low-pass filter bias insertion unit 3-, 6-, 10-, and 20-dB attenuators adjustable attenuator rotary joint coupling capacitor 10-, 20-, and 30-cm rigid air lines 33-58 cm adjustable line constant-Z adjustable lines radiating line trombone constant-Z line	ML MB MR, MRL R20A, R20LA R22A, R22LA R33, R34 T, TL TPD, TPDL U UBL VCL VI VQ, VQL VR, VRL W100 W200 W50B, W50BL WN, WN3 WO, W03 X• XL Y Z	component mount coupling probe mixer-rectifier patch cord, double shield patch cord, double shield patch cord, single shield tee power divider U-line section balun variable capacitor voltmeter indicator voltmeter detector voltmeter rectifier 100-Ω termination 200-Ω termination 50-Ω termination short-circuit terminations insertion unit series inductor cliplock stand

MISCELLANEC	OUS COAXIAL C	UNNECTURS
CONNECTOR TYPE	TYPE NO.	USED WITH
Basic	874-B	50-ohm Air Line
Basic Locking	87 4-BB L	50-ohm Air Line
Panel Locking	874-PLT	Wire Lead
Panel Locking Recessed	874-PRLT	Wire Lead
Panel Locking Feedthrough	874-PFL	Type 874 Patch Cords

L suffix indicates locking Type 874 Connector.

FOR COMPLETE DETAILS, REFER TO THE GENERAL RADIO CATALOG.

GENERAL RADIO COMPANY

WEST CONCORD, MASSACHUSETTS 01781

617 369-4400

617 646-7400

SALES ENGINEERING OFFICES

NEW ENGLAND*

22 Baker Avenue West Concord, Massachusetts 01781 Telephone 617 646-0550

METROPOLITAN NEW YORK*

Broad Avenue at Linden
Ridgefield, New Jersey 07657
Telephone N.Y. 212 964-2722
N.J. 201 943-3140

SYRACUSE

Pickard Building
East Molloy Road
Syracuse, New York 13211
Telephone 315 454-9323

PHILADELPHIA

Fort Washington Industrial Park Fort Washington, Pennsylvania 19034 Telephone 215 646-8030

WASHINGTON* AND BALTIMORE

11420 Rockville Pike Rockville, Maryland 20852 Telephone 301 946-1600

ORLANDO

113 East Colonial Drive Orlando, Florida 32801 Telephone 305 425-4671

* Repair services are available at these district offices.

CHICAGO*

6605 West North Avenue Oak Park, Illinois 60302 Telephone 312 848-9400

CLEVELAND

5579 Pearl Road Cleveland, Ohio 44129 Telephone 216 886-0150

LOS ANGELES*

1000 North Seward Street Los Angeles, California 90038 Telephone 213 469-6201

SAN FRANCISCO

626 San Antonio Road Mountain View, California 94040 Telephone 415 948-8233

DALLAS*

2600 Stemmons Freeway, Suite 210 Dallas, Texas 75207 Telephone 214 637-2240

TORONTO*

99 Floral Parkway Toronto 15, Ontario, Canada Telephone 416 247-2171

MONTREAL

1255 Laird Boulevard

Town of Mount Royal, Quebec, Canada

Telephone 514 737-3673

General Radio Company (Overseas), 8008 Zurich, Switzerland General Radio Company (U.K.) Limited, Bourne End, Buckinghamshire, England Representatives in Principal Overseas Countries

Printed in USA